

02-18-00

H

JCS71 U.S. PTO
02/16/00

Please type a plus sign (+) inside this box [+]

PTO/SB/05 (12/97)

Approved for use through 09/30/00. OMB 0651-0032

Patent and Trademark Office: U.S. DEPARTMENT OF COMMERCE

Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.

JCS82 U.S. PTO
09/30/00
02/16/00

UTILITY PATENT APPLICATION TRANSMITTAL
(Only for new nonprovisional applications under 37 CFR 1.53(b))

Attorney Docket No. 003764.P025 Total Pages 2

First Named Inventor or Application Identifier Jessica Chiu, et al.

Express Mail Label No. EL 512 770 225 US

ADDRESS TO: Assistant Commissioner for Patents
Box Patent Application
Washington, D. C. 20231

APPLICATION ELEMENTS
See MPEP chapter 600 concerning utility patent application contents.

1. X Fee Transmittal Form
(Submit an original, and a duplicate for fee processing)

2. X Specification (Total Pages 118)
(preferred arrangement set forth below)
- Descriptive Title of the Invention
- Cross References to Related Applications
- Statement Regarding Fed sponsored R & D
- Reference to Microfiche Appendix
- Background of the Invention
- Brief Summary of the Invention
- Brief Description of the Drawings (if filed)
- Detailed Description
- Claims
- Abstract of the Disclosure

3. X Drawings(s) (35 USC 113) (Total Sheets 20)

4. X Oath or Declaration (Total Pages 5) (unsigned)
a. Newly Executed (Original or Copy)
b. Copy from a Prior Application (37 CFR 1.63(d))
(for Continuation/Divisional with Box 17 completed) (**Note Box 5 below**)
i. **DELETIONS OF INVENTOR(S)** Signed statement attached deleting
inventor(s) named in the prior application, see 37 CFR 1.63(d)(2)
and 1.33(b).

5. Incorporation By Reference (useable if Box 4b is checked)
The entire disclosure of the prior application, from which a copy of the oath or
declaration is supplied under Box 4b, is considered as being part of the
disclosure of the accompanying application and is hereby incorporated by
reference therein.

6. Microfiche Computer Program (Appendix)

00506094 021500

7. _____ Nucleotide and/or Amino Acid Sequence Submission
(if applicable, all necessary)
a. _____ Computer Readable Copy
b. _____ Paper Copy (identical to computer copy)
c. _____ Statement verifying identity of above copies

ACCOMPANYING APPLICATION PARTS

8. _____ Assignment Papers (cover sheet & documents(s))
9. _____ a. 37 CFR 3.73(b) Statement (where there is an assignee)
_____ b. Power of Attorney
10. _____ English Translation Document (if applicable)
11. _____ a. Information Disclosure Statement (IDS)/PTO-1449
_____ b. Copies of IDS Citations
12. _____ Preliminary Amendment
13. X Return Receipt Postcard (MPEP 503) (Should be specifically itemized)
14. _____ a. Small Entity Statement(s)
_____ b. Statement filed in prior application, Status still proper and desired
15. _____ Certified Copy of Priority Document(s) (if foreign priority is claimed)
16. X Other: Copy of postcard with Express Mail label

17. **If a CONTINUING APPLICATION**, check appropriate box and supply the requisite information:
____ Continuation ____ Divisional ____ Continuation-in-part (CIP)
of prior application No: _____

18. Correspondence Address

____ Customer Number or Bar Code Label _____
(Insert Customer No. or Attach Bar Code Label here)
or
X Correspondence Address Below
NAME Darren J. Milliken, Reg. No. 42,004 2/16/00
BLAKELY, SOKOLOFF, TAYLOR & ZAFMAN LLP
ADDRESS 12400 Wilshire Boulevard
Seventh Floor
CITY Los Angeles STATE California ZIP CODE 90025-1026
Country U.S.A. TELEPHONE (408) 720-8598 FAX (408) 720-9397

12/01/97

- 2 -

PTO/SB/05 (12/97)

Approved for use through 09/30/00. OMB 0651-0032
Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE

009120-10000000

UNITED STATES PATENT APPLICATION

for

**MULTI-LUMEN FLUTED BALLOON RADIATION CENTERING
CATHETER**

Inventors:

Eric D. Peterson
Manolo F. Lumauig
Jessica Chiu

prepared by:

BLAKELY, SOKOLOFF, TAYLOR & ZAFMAN
12400 Wilshire Boulevard
Seventh Floor
Los Angeles, California 90025-1026


Docket No.: 003764.P025

"Express Mail" mailing label number: EL512770225US

Date of Deposit: February 16, 2000

I hereby certify that I am causing this paper or fee to be deposited with the United States Postal Service "Express Mail Post Office to Addressee" service on the date indicated above and that this paper or fee has been addressed to the Assistant Commissioner for Patents, Washington, D. C. 20231

Beatrice Orozco
(Typed or printed name of person mailing paper or fee)

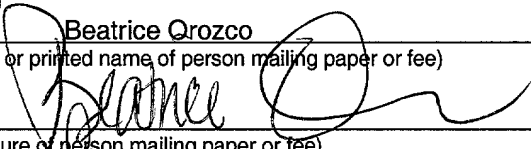
(Signature of person mailing paper or fee)

February 16, 2000
(Date signed)

003764.P025

MULTI-LUMEN FLUTED BALLOON RADIATION CENTERING CATHETER

BACKGROUND OF THE INVENTION

5 Field of the Invention

The present invention relates to medical catheters and more particularly to a multi-lumen balloon for a radiation centering catheter.

Description of Related Art

Medical catheters generally include elongate tube-like members that may be
10 inserted into the body, either percutaneously or via a body orifice, for any of a wide variety of diagnostic and interventional purposes. Such catheters are particularly useful with regard to certain cardiovascular applications where the object is to deliver a treatment or instrument to a remote lesion.

Percutaneous Transluminal Coronary Angioplasty (PTCA or balloon
15 angioplasty) is the predominant treatment for coronary vessel stenosis. In PTCA, catheters are inserted into the cardiovascular system via the femoral artery under local anesthesia. A pre-shaped guiding catheter is positioned in the coronary artery, and a dilatation catheter having a distensible balloon portion is advanced through the guiding catheter into the branches of the coronary artery until the
20 balloon portion traverses or crosses a stenotic lesion. The balloon portion is then inflated with a medium to compress the atherosclerosis in a direction generally perpendicular to the wall of the artery, thus dilating the lumen of the artery. Patients treated by PTCA procedures, however, suffer from a high incidence of restenosis, i.e., the same area of the coronary vessel collapses or becomes obstructed.

Recent preclinical and early clinical studies indicate that intravascular radiation after balloon angioplasty can reduce the rate of restenosis caused by intimal hyperplasia. Generally, in an intravascular radiotherapy procedure, a flexible catheter is inserted into the cardiovascular system of a patient and then advanced
5 to the region of the vessel that has been subjected to the angioplasty procedure. A radiation source or a treatment catheter having a radiation source inside it is then advanced through the flexible catheter so that the radiation source reaches the stenosed vascular site and can deliver an effective dose of radiation. After the radiation treatment, the catheter and radiation source are removed.

10 Because for a given radiation source activity, the intensity of the radiation delivered to a vessel wall varies in inverse proportion to the square of the distance between the radiation source and the vessel wall, it is desirable to hold the radiation source at, or reasonably near, the center of the vessel for a given treatment period. If the source is not centered within vessel, the vessel wall nearest the source may
15 receive an excess of radiation, while the portion of the vessel wall farthest from the source may be underexposed to the radiation.

There are a number of ways to center a radiation source within a vessel. One such way is using a spiral balloon having a central lumen in which the radiation source is advanced to the stenosed vessel site. In a spiral balloon catheter, the
20 balloon is wrapped or molded in a spiral fashion around a flexible centering lumen. When inflated, the balloon outer diameter pushes against the vessel walls while the

inner balloon diameter pushes the radiation source lumen toward the center of the vessel.

Spiral balloons have several significant drawbacks when used in intervascular radiotherapy to control restenosis. The first drawback is that because
5 the balloon is wrapped or molded in a spiral shape around the centering lumen of the catheter, the centering effect of the radiation source decreases as the pitch of the turns of the spiral balloon increases. Thus, the fewer turns a spiral balloon has in its configuration, the less centered the radiation source is inside the vessel. Also, if the spiral balloon is over-pressurized, it will lose its spiral shape, thus leading to
10 inconsistent centering of the radiation source. Another drawback with a spiral balloon is that because every spiral is a taper, when the balloon is in a deflated configuration, it creates a stiff catheter with a bulky balloon. This leads to poor access and limits the use of spiral catheters to certain portions of the vascular system. Furthermore, at the end of the intervascular radiation procedure, the tapers
15 create poor refold of the spiral thus making the removal of the balloon catheter difficult for the physician. Another significant disadvantage of using a spiral balloon in intervascular radiation is the spiral balloon's inconsistent blood perfusion ability. Good blood perfusion of the vessel is achieved only when the blood is flowing freely through the spiral cavity created by the balloon. If any portion of the spiral cavity is
20 blocked, then the flow of the blood is also stopped at that point. Thus, blood perfusion may not be adequate.

Another way to center a radiation source within a vessel is to use a segmented balloon catheter having a series of peaks and valleys created by segmenting an ordinary balloon catheter. The segmented balloon centers the centering lumen using the same principle as the spiral balloon catheter.

5 An additional way to center a radiation source within a vessel is by using a catheter having an outer balloon and an inner balloon disposed within the outer balloon. Generally, the inner and outer balloons are positioned parallel to each other and axially with the catheter shaft. The inner and outer balloons may have a spiral or a segmented configuration. The inner centering balloon may also be a
10 multiple axial lumen balloon, where the lumens extend parallel to the catheter shaft.

Another way to center a radiation source within a vessel is by having a balloon attached to the distal portion of a radioguide catheter. When inflated, the balloon engages the walls of the vessel to center the treatment channel. The balloon may also be configured to include spiral lumens or/and perfusion lumens to
15 permit perfusion of the blood when the balloon is inflated.

Segmented balloon catheters and multiple balloon catheters have many of the same drawbacks as those associated with spiral balloon catheters, including inadequate centering of the radiation source, poor balloon refold, catheter stiffness, bulky balloon configuration, inconsistent perfusion, etc. While balloons configured
20 with spiral lumens or perfusion lumens have a better perfusion capability than single-spiral, segmented, or multiple balloon configurations, they still have some

disadvantages, including poor balloon foldability, catheter stiffness, and less than optimal perfusion capability.

Currently, most radioguide centering catheters used in the industry are of the type known in the industry as “tip RX” (RX being “rapid exchange”). Tip RX radioguide centering catheters are characterized by a short guidewire riding length of approximately 5 mm and a guidewire exit notch distal to the centering balloon. Tip RX catheter assemblies have several disadvantages when used in vascular radiation therapy. First, the trackability of the catheter is not consistent in a challenging vascular anatomy, and can go from excellent to poor for no apparent reason. Poor catheter trackability may make it impossible to place the catheter at the desired treatment site, preventing delivery of the radiation therapy. Pushability is similarly problematic with the tip RX catheter. When withdrawing a tip RX catheter, it is also possible to prolapse the guidewire, complicating the procedure. Another disadvantage is that because the guidewire lumen is distal to the balloon, it adds approximately 10 mm to the overall length of the tip. Cardiologists however, prefer to have the tip of the catheter as short as possible in order to prevent potential injury to the artery distal to the treatment site. Another disadvantage of using a tip RX balloon catheter for vascular radiation therapy is that since the exit notch is distal to the balloon, the guidewire must be left in place, thus creating a small but measurable shadow in the radiation dosimetry.

In addition to tip RX balloon catheters, other catheter designs used for vascular radiotherapy employ an “over-the-wire” (“OTW”) guidewire lumen

configuration. Currently, these OTW radiation delivery catheters do not provide the capability of centering the radiation source. Furthermore, while an over-the-wire configuration catheter assembly allows for the guidewire to be pulled back during radiation delivery, the guidewire lumen shifts the source away from the center of the catheter, thus making the centering of the radiation source even more problematic.

The manufacture of inflated balloons with diameters in a range of approximately 1.0 to 6.0 millimeters (mm) presents another significant issue with current balloon catheter designs. One of the challenges relates to the stiffness of the balloon. For example, some manufacturers have used several separate small diameter balloons and attached them using glue or other bonding material around a central catheter shaft to form a balloon catheter. Because the glue or bonding material is positioned along the catheter shaft, the catheter is stiff and difficult to use in coronary vessels having tortuous paths. Therefore, this design configuration gives sub-par performance. Others have used an extrusion process to manufacture a multiple balloon radiation centering catheter. During the extrusion process, however, excess material is generated which tends to make the catheter stiff. In addition, because the material used for the radiation source lumen has generally been different than the material used for the guidewire lumen or the centering balloons, the extrusion process is extremely difficult to complete successfully.

SUMMARY OF THE INVENTION

A multi-lumen balloon designed for a radiation centering catheter and method for manufacturing the same is described. One embodiment of the present invention is a multi-lumen balloon radiation centering catheter assembly that includes a catheter shaft and a multi-lumen balloon disposed at the distal end of the shaft. The multi-lumen balloon has a plurality of inflatable outer lumens disposed around a central lumen, the outer lumens integrally coupled with the central lumen so as to form the multi-lumen balloon. The catheter shaft includes an inner lumen longitudinally extending through at least a portion of the catheter shaft proximate the balloon and connected to the central lumen of the balloon. The shaft inner lumen is adapted for receiving a radiation source lumen. The shaft inner lumen is further adapted to receive a guidewire lumen for positioning the multi-lumen balloon radiation centering catheter within the body vessel. The guidewire lumen extends lengthwise through one of the outer lumens of the multi-lumen balloon.

A second embodiment of the present invention is a multi-lumen balloon radiation centering catheter assembly, which includes a multi-lumen balloon having a plurality of outer lumens disposed around a central lumen and a catheter shaft disposed proximate the balloon. The outer lumens are integrally coupled with the central lumen so as to form the multi-lumen balloon having a slideable proximal seal and a slideable distal seal. The catheter shaft includes an inner lumen longitudinally extending through at least a portion of the catheter shaft proximate to the balloon and connected to the central lumen of the balloon. The inner tubular

member is adapted for receiving a radiation source lumen and a guidewire for positioning the multi-lumen balloon radiation centering catheter within a body vessel. The inner tubular member further includes an inflation lumen that is in fluid communication with the balloon outer lumens to allow an inflation medium to enter
5 and inflate the plurality outer lumens so as to cause the radiation source lumen to be centered within a body vessel.

A third embodiment of the present invention is a multi-lumen balloon radiation centering catheter assembly, which includes a multi-lumen balloon having a plurality of inflatable outer lumens disposed around a central lumen and a catheter
10 shaft disposed proximate the balloon. The outer lumens are integrally coupled with the central lumen so as to form the multi-lumen balloon having a proximal seal and a distal seal. The balloon further includes a plurality of bores communicating between the central lumen and the plurality of outer lumens. The catheter shaft includes an inner tubular member that extends coaxially within an outer tubular
15 member, the inner tubular member adapted for receiving a radiation source lumen. The inner tubular member further includes an inflation lumen that is in fluid communication with the balloon central lumen and the plurality of outer lumens to allow an inflation medium to enter and inflate the outer lumens so as to cause the radiation source lumen to be centered within a body vessel.

BRIEF DESCRIPTION OF THE DRAWINGS

The present invention is illustrated by way of example and not limitation in the accompanying figures:

5 FIG. 1 is a side view of one embodiment of a multi-lumen fluted balloon catheter assembly for centering a radiation source, with guidewire lumen extending through one of the outer lumens of the balloon.

10 FIG. 2 is a cross-sectional view of the multi-lumen fluted balloon catheter assembly of FIG. 1 taken along line A--A.

 FIG. 3 is a cross-sectional view of the multi-lumen fluted balloon radiation centering catheter assembly of FIG. 1 taken along line B--B.

15 FIG. 4 is a cross-sectional view of the multi-lumen fluted balloon radiation centering catheter assembly of FIG. 1 taken along line C--C.

 FIG. 5 is a cross-sectional view of the multi-lumen fluted balloon radiation centering catheter assembly of FIG. 1 taken along line D--D.

20

FIG. 6 is a side view of a second embodiment of a multi-lumen fluted balloon catheter assembly (standard-RX configuration) for centering radiation source, with proximal and distal slideable seals and without a guidewire lumen.

FIG. 7 is a cross-sectional view of the multi-lumen fluted balloon radiation
5 centering catheter assembly of FIG. 6 taken along line E--E.

FIG. 8 is a cross-sectional view of the multi-lumen fluted balloon radiation centering catheter assembly of FIG. 6 taken along line F--F.

10 FIG. 9 is a cross-sectional view of the multi-lumen fluted balloon radiation centering catheter assembly of FIG. 6 taken along line G--G.

FIG. 10 is a side view of a third embodiment of the multi-lumen fluted balloon catheter assembly (for a tip-RX configuration) for centering a radiation source.

15 FIG. 11 is a cross-sectional view of the multi-lumen fluted balloon catheter assembly of FIG. 10 taken along line H--H.

FIG. 12 is a partial longitudinal cross-sectional view of the multi-lumen fluted
20 balloon catheter assembly of FIG. 10 taken along line J--J showing a configuration for inflation/deflation and attachment.

FIG. 13 is a side view of an third embodiment of a multi-lumen fluted balloon catheter assembly (for a standard-RX configuration) for centering a radiation source, where the guidewire lumen and source lumen extend through catheter inner member and central balloon lumen.

5

FIG. 14 is a cross-sectional view of the multi-lumen fluted balloon catheter assembly of FIG. 13 taken along line K—K showing a guidewire lumen extending through balloon central lumen.

10

FIG. 15 is a cross-sectional view of the multi-lumen fluted balloon catheter assembly of FIG. 13 taken along line L—L showing guidewire lumen, radiation source lumen, and inflation/deflation lumen within catheter inner member.

15

FIG. 16 is a cross-sectional view of the multi-lumen fluted balloon catheter assembly of FIG. 13 taken along line M—M showing guidewire lumen and radiation source lumen.

20

FIG. 17 is a schematic side view of the proximal and distal balloon seal areas for the fluted balloon radiation centering catheter assembly of FIG. 1.

FIG. 18 is a cross-sectional view of a four-lumen balloon for a centering catheter assembly.

FIG. 19a is a cross-sectional view of the four-lumen balloon for a centering catheter assembly with two balloon outer lumens flattened for proximal balloon seal preparation.

5

FIG. 19b is a cross-sectional view of the four-lumen balloon for a centering catheter assembly with a configuration for folding the two balloon outer lumens flattened for balloon proximal seal preparation.

10 FIG. 19c is a cross-sectional view of the four-lumen balloon for a centering catheter assembly with another configuration for folding the two balloon outer lumens flattened for balloon proximal seal preparation.

15 FIG. 20a is a cross-sectional view of a configuration for a completed balloon proximal seal for a four-lumen balloon.

FIG. 20b is a cross-sectional view of a second configuration for a completed balloon proximal seal for a four-lumen balloon.

20 FIG. 20c is a cross-sectional view of a third configuration for a completed balloon proximal seal for a four-lumen balloon.

FIG. 20d is a side view of a “football-shape” cross section mandrel used to perform the proximal seal for a multi-lumen balloon.

FIG. 21a is a schematic side view of the distal balloon seal area for the multi-lumen fluted balloon radiation centering catheter assembly of FIG. 1.

FIG. 21b is a schematic side view of the tip-forming sheath for forming the tip of balloon distal seal for the multi-lumen fluted balloon radiation centering catheter assembly of FIG. 1.

10

FIG. 21c is a schematic side view of the first and second heat shrink tube materials used for the balloon distal seal.

15

FIG. 21d is a schematic side view of the source mandrel having a tapered length.

FIG. 21e shows schematic side, top and bottom views of the source mandrel having a ramp length.

20

FIG. 22a is a cross-sectional view of a basic four-lumen (quad-lumen) extrusion tubing with “shared wall” and “fillet radius” regions.

FIG. 22b is a cross-sectional view of a tip and die assembly used to make the quad-lumen extrusion tubing of FIG. 22a.

FIG. 23a is a cross-sectional view of a second embodiment of a quad-lumen
5 extrusion tubing with “shared wall” and “undercut” regions.

FIG. 23b is a cross-sectional view of a tip and die assembly used to make the quad-lumen extrusion tubing of FIG. 23a.

10 FIG. 24a is a cross-sectional view of a third embodiment of a quad-lumen extrusion tubing with “shared wall” and “undercut” regions.

FIG. 24b is a cross-sectional view of a tip and die assembly used to make the quad-lumen extrusion tubing of FIG. 24a.

15 FIG. 25a is a cross-sectional view of a fourth embodiment of a quad-lumen extrusion tubing with “standoffs” regions.

FIG. 25b is a cross-sectional view of a tip and die assembly used to make
20 the quad-lumen extrusion tubing of FIG. 25a.

FIG. 26 is a flow chart illustrating a method of manufacture a multi-lumen balloon assembly of the present invention.

FIG. 27a is a side view of another embodiment of a multi-lumen fluted balloon catheter assembly for centering radiation source, with two additional
5 guidewire exits in the catheter shaft and guidewire extending longitudinally outside the balloon.

FIG. 27b is a cross-sectional view of the multi-lumen fluted balloon radiation
10 centering catheter assembly of FIG. 27a taken along line A--A.

FIG. 27c is a cross-sectional view of the multi-lumen fluted balloon radiation centering catheter assembly of FIG. 27a taken along line B--B.

15 FIG. 27d is a cross-sectional view of the multi-lumen fluted balloon radiation centering catheter assembly of FIG. 27a taken along line C--C.

DETAILED DESCRIPTION OF THE INVENTION

A multi-lumen balloon for use in a fluted balloon centering catheter and method for providing the same is described. The present invention is a multi-lumen balloon for a radiation centering catheter that maintains a radiation source at the center of a cardiovascular artery, has improved blood perfusion capability, and has improved balloon refolding characteristics. The present invention also provides an improved method of manufacture for a multi-lumen balloon design for a radiation centering catheter, where such method allows the manufacture of the multi-lumen balloon sub-assembly to be done separately from the catheter shaft assembly. Furthermore, the present invention is a multi-lumen balloon centering catheter assembly with an improved guidewire design and method for providing the same. In addition, the present invention provides improved proximal and distal balloon seal designs and method of manufacture for the same.

In the following detailed description, numerous specific details are set forth in order to provide a more thorough understanding of the present invention. However, it will be apparent to those skilled in the art to which this invention pertains that the present invention may be practiced without these specific details. In other instances, well-known devices, methods, procedures, and individual components have not been described in detail so as not to unnecessarily obscure aspects of the present invention.

The present invention is a multi-lumen fluted balloon radiation centering catheter. FIG. 1 shows an embodiment of the multi-lumen fluted balloon centering

catheter assembly 1 of the present invention that includes a multi-lumen balloon 10 and an interventional catheter 2 disposed at the proximal end of the balloon 10.

1 Balloon 10 includes a central lumen and a plurality of outer lumens (or lobes) disposed around the central lumen. The outer lumens are integrally coupled with
5 the central lumen so as to form the multi-lumen balloon. It should be noted that although the multi-lumen balloon configurations illustrated and discussed hereafter make reference to a four-lumen balloon configuration (i.e., balloon with a central lumen and three outer lumens), the multi-lumen balloon of the present invention is not limited to this four-lumen balloon arrangement. As it will be described in the
10 later sections, for some treatment applications and/or vessel treatment area configurations, using a three-lumen balloon having a central lumen and two outer lumens may be desirable. In addition, for some applications, having a balloon with more than four lumens may be desirable.

The interventional catheter 2 used with the multi-lumen balloon 10 may be
15 one of several configurations known in the art, including a standard Rapid Exchange ("RX") design (as shown in side views in FIGS. 1 and 13) where a guidewire lumen 21 passes through the balloon 10 and exits proximal to the balloon 10; a tip (or distal) RX design (as shown in a side view in FIG. 10) where a short guidewire lumen 21 is provided at a distal tip of the balloon 10; or an over-the-wire
20 ("OTW") design where the guidewire lumen 21 extends the full length of the fluted balloon catheter assembly 1, including the multi-lumen balloon 10 and interventional catheter 2.

Multi-lumen Balloon

Referring to FIG. 18, a cross sectional view of one embodiment of a multi-lumen balloon 10 for treating a body vessel 16 in the vascular system is shown. Balloon 10 includes a central lumen 12 and a plurality of outer lumens (or lobes) 11 disposed around the central lumen 12. The outer lumens 11 are integrally coupled with the central lumen 12 so as to form the multi-lumen balloon 10. Each of the balloon outer lumens 11 has an inner radial length (or diameter) 18 and an outer diameter 15, defining balloon outer lumen walls 17. The walls 17 of balloon outer lumens 11 are made very thin to allow proper inflation and deflation of outer lumens 11. The thickness of the walls 17 ranges from 0.5/1000 in. to about 3/1000 in. In one embodiment, wall 17 has a thickness of 0.75/1000 in.

The balloon outer lumens 11 can be extruded with either equal diameters 15 (as shown in FIG. 18, and FIGS. 3 and 11) or with unequal (i.e., asymmetrical, lopsided, etc.) diameters 15 (as shown in FIG. 14). The balloon outer lumen has a diameter 15 sized in a range of approximately 0 mm (no balloon lumen) to about 5 mm.

The balloon central lumen 12 has an inner diameter 18a. The central lumen 12 is capable of containing a radiation source (with or without a radiation source lumen) therein. The diameter 18a of the balloon central lumen 12 is sized based on the radiation source outer diameter, for example a radiation source wire having an outer diameter in a range of approximately 10/1000 in. to 50/1000 in. It should be noted that the balloon central lumen diameter 18a may be made smaller than

18/1000 in. for intervascular radiation treatments using radiation sources having a diameter smaller than 10/1000 in. or for radiation sources having a liquid configuration.

Continuing with reference to FIG. 18, the multi-lumen balloon 10 of the present invention is used in a fluted balloon radiation centering catheter assembly 1 for treating a body vessel 16 in the vascular system. Given the very small diameter of these body vessels 16, the combined balloon diameter 13 (as measured across all balloon outer lumens 11 while balloon is in an inflated or deployed state) is kept in a range of approximately 1.5 mm to 6 mm for coronary vessels and in a range of approximately 3 mm to 12 mm for peripheral vessels. In one embodiment (shown in FIG. 3), the combined diameter 13 is in a range of approximately 1.5 mm to 4 mm.

Referring now to FIG. 3, another embodiment of the multi-lumen balloon of this invention includes a balloon 10 having a central lumen 12 and three outer lumens (or lobes) 11 disposed around the central lumen 12. The outer lumens 11 are integrally coupled with the central lumen 12 so as to form the multi-lumen balloon 10. Balloon 10 has a guidewire lumen 21 extending lengthwise through one of the balloon outer lumens 11. The guidewire lumen 21 is capable of receiving a guidewire 45 for positioning the multi-lumen balloon 10 (and thus the radiation centering catheter 1) within a body vessel 16. The balloon central lumen 12 is capable of containing a radiation source 25 (with or without a radiation source lumen 22) therein. If a radiation source lumen 22 is used with the radiation source

25 in the balloon central lumen 12, the radiation source lumen 22 would extend lengthwise through the central lumen 12.

It should be noted that the multi-lumen balloon embodiment shown in FIG. 3 is also adapted for receiving the guidewire lumen 21 (with a guidewire 45) through its central lumen 12. In this configuration, since the balloon central lumen 12 would contain both a radiation source 25 (with or without a radiation source lumen 22) and a guidewire lumen 21, the central lumen 12 may take an egg-like shape. The inner diameter 18a of the egg-shaped central lumen 12 would be sized based on the diameter of the radiation source 25 (with its radiation source lumen 22 if one is present) and the diameter of the guidewire lumen 21. In this configuration, the diameter 18a of the balloon central lumen 12 is sized based on the radiation source outer diameter, for example a radiation source wire having an outer diameter in a range of approximately 10/1000 in. to 50/1000 in., and the guidewire lumen diameter. Thus, the diameter 18a may be in a range of approximately 10/1000 in. to 75/1000 in. In one embodiment, the diameter 18a is 62/1000 in.

With reference to FIG. 4, for the four-lumen balloon embodiment shown in FIG. 3, three separate inflation lumens (54b, 55b) positioned proximal to the balloon 10 in a catheter shaft 41 are used to inflate the three balloon outer lumens 11. The inflation lumens (54b, 55b) communicate directly with each of the balloon outer lumens 11. A common inflation lumen 36, positioned within the catheter shaft outer member 46 (shown in FIG. 5), provides a common communication path between the inflation lumens (54b, 55b) (and thus the balloon outer lumens 11) and an

inflation port 33 (shown in FIG. 1) to which a balloon inflation means (not shown) is attached. In this configuration, an inflation medium 18b enters the balloon catheter assembly at the inflation port 33, passes through the common inflation lumen 36 onto the three balloon inflation lumens (54b, 55b), and then enters and inflates the
5 outer lumens 11 which causes the radiation source lumen 22 (and/or radiation source 25) to be centered within the body vessel 16. The outer lumens 11 may be inflated at an operating pressure in a range of approximately 0.5-14 atmospheres. In one embodiment, the outer lumens 11 may be inflated at an operating pressure in a range of approximately 2-5 atmospheres.

10 For the multi-lumen balloon shown in FIG. 3, the central lumen 12 does not have to be pressurized and may not have to be sealed in order to inflate the balloon outer lumens 11. It should be noted that having individual inflation lumens for each of the balloon outer lumens allows each balloon outer lumen to be inflated to different pressures. This multi-lumen balloon arrangement is desirable for vessel
15 treatment applications where the particular body vessel (in the area being treated) may not be fully circular (i.e., body vessel area may contain certain obstructions or “deposits” along its walls).

It should also be noted that it is not necessary to have individual inflation lumens (54b, 55b) for each of the balloon outer lumens 11 in order to center to
20 radiation source lumen 22 with the vessel 16. For balloon designs where individual inflation lumens (54b, 55b) are absent, a catheter shaft inner lumen 41a may serve as a common inflation lumen for the balloon outer lumens 11.

Continuing with reference to FIG. 3, the diameter 18a of the balloon central lumen 12 is sized based on the radiation source outer diameter, for example a radiation source wire having an outer diameter in a range of approximately 10/1000 in. to 50/1000 in. The combined balloon diameter 13 (as measured across all balloon outer lumens 11 while balloon is in an inflated or deployed state) is kept in a range of approximately 1.5 mm to 6 mm for coronary vessels and in a range of approximately 3 mm to 12 mm for peripheral vessels. For the embodiment shown in FIG. 3, a balloon having a combined diameter 13 in a range of approximately 1.5 mm to 4 mm is advantageous when treating coronary vessels.

Referring to FIG. 11, another embodiment of the multi-lumen balloon of this invention is a balloon 10 having a central lumen 12 and a plurality of outer lumens 11 disposed around the central lumen 12. The outer lumens 11 are integrally coupled with the central lumen 12 so as to form the multi-lumen balloon 10. Bores (or channels) 35 are formed between the outer lumens 11 and the central lumen 12. This arrangement allows an inflation medium 18b to pass from the balloon central lumen 12 into the outer lumens 11 and inflate outer lumens 11, causing a radiation source lumen 22 to be centered within a body vessel 16. In this configuration, the central lumen 12 may have to be pressurized in order for the outer lumens 11 to properly inflate and center the radiation source lumen 22 within the body vessel 16.

For the balloon configuration shown in FIG. 11, the balloon central lumen 12 is capable of containing a radiation source 25 (with or without a radiation source lumen 22) therein. The multi-lumen balloon embodiment shown in FIG 11 is

adapted for receiving a guidewire lumen (with a guidewire) through either one of its balloon outer lumens 11 or through its central lumen 12. Because in FIG. 11 the balloon 10 is shown as being used with a tip (or distal) Rapid Exchange catheter type (i.e., the guidewire is positioned distal to the balloon), for the balloon embodiment of FIG. 11, the guidewire does not extend through any of the balloon lumens 11.

It should be noted that while the balloon configuration of FIG. 3 shows a guidewire lumen 21 (with guidewire 45) extending through one of the balloon outer lumens 11, the guidewire 45 (with or without its guidewire lumen 21) may also be positioned so that it extends through the central lumen 12 of the multi-lumen balloon 10 (as shown in the balloon configuration of FIG. 14). Furthermore, whether a guidewire (and a guidewire lumen) extends through the multi-lumen balloon depends on a number of considerations, such as the type of catheter used, the balloon catheter manufacturing preferences, the treatment site configuration, etc. For example, when considering the type of catheter to be used, for a standard Rapid Exchange or an OTW catheter type, the guidewire 45 (with or without a guidewire lumen 21) would extend through one of the outer lumens (as shown in FIGS. 3, 6, and 17) or through the central lumen (as shown in FIG. 14). For balloon catheter assemblies using a tip (or distal) Rapid Exchange catheter type, because the guidewire (with or without a guidewire lumen) is positioned distal to the balloon, the guidewire would not extend through any of the balloon lumens (as shown in FIG. 11).

As with the other two balloon arrangements discussed above, for the balloon embodiment shown in FIG. 11 (i.e., having a “tip” or distal guidewire lumen that does not extend through the entire balloon lumen), the diameter 18a of the balloon central lumen 12 is sized based on the radiation source outer diameter, for example a radiation source wire having an outer diameter in a range of approximately 10/1000 in. to 50/1000 in. For the balloon embodiment shown in FIG. 14 (i.e., where the guidewire lumen 21 is positioned so that it extends through the central lumen 12), the diameter 18a of the balloon central lumen 12 is sized based on the radiation source outer diameter and the diameter of the guidewire lumen 21. Thus, the diameter 18a may be in a range of approximately 10/1000 in. to 75/1000 in. In one embodiment, the diameter 18a is 62/1000 in.

Continuing with reference to FIG. 11, the combined balloon diameter 13 (as measured across all balloon outer lumens 11 while balloon is in an inflated or deployed state) is kept in a range of approximately 1.5 mm to 6 mm for coronary vessels and in a range of approximately 3 mm to 12 mm for peripheral vessels. For the embodiment shown in FIG. 11, a balloon having a combined diameter 13 in a range of approximately 1.5 mm to 4 mm is desirable when treating coronary vessels.

Referring now to FIG. 17, a four-lumen balloon 10 having a guidewire lumen 21 extending through one of the balloon outer lumens 11 is shown. Note that one of the outer lumens is hidden from view. A radiation source lumen 22 (capable of holding a radiation source) extends lengthwise through the balloon central lumen

12. The outer lumen 11 with the guidewire lumen 21 extending through it is also inflated as part of the function of the centering balloon catheter.

Continuing with reference to FIG. 17, the multi-lumen balloon 10 has a distal seal 28 and a proximal seal 29. Distal seal 28 seals the plurality of distal ends 34b of the balloon outer lumens 11 to a catheter shaft (formed by the radiation source lumen 22 and guidewire lumen 21) while the proximal seal 29 seals the plurality of proximal ends 34a of the balloon outer lumens 11 to the catheter shaft. The distal and proximal seals (28, 29) may each have a width in a range of approximately 0.5 mm to about 5 mm.

When balloon outer lumens' distal and proximal ends (34b, 34a) are sealed together into the distal seal and proximal seal respectively (28, 29), each of the outer lumens 11 takes the form of a "flute" (i.e., an elongated cylinder having tapered ends) when inflated by an inflation medium. The fluted balloon configuration shown in FIG. 17 is representative of balloon configurations of this invention (as shown in balloon catheter assemblies of FIGS. 1, 6, 10, and 13).

Referring to FIG. 1, a treatment area 30 is defined between the balloon's distal seal 28 and proximal seal 29. The longitudinal length of the balloon treatment area 30 is made to be appropriate for the body vessel to be treated (for example, coronary vessels or peripheral vessels) and for the radiation treatment to be delivered. In one embodiment of the present invention, the balloon treatment area length 30 is in a range of approximately 18 mm to 54 mm. For some intervascular gamma radiation treatments, such as treatments on peripheral vessels of the

cardiovascular system, the balloon treatment area length 30 may be in a range of approximately 10 mm to 250 mm.

Referring now to FIG. 3, during vascular radiotherapy, when inflated and engaged with the walls of the body vessel 16, the balloon outer lumens 11 define a series of straight longitudinal paths 14 that allow for perfusion of blood (not shown) past balloon treatment area 30 (shown in FIG. 1).

The fluted balloon outer lumens 11 can be extruded with either equal diameter 15 (as shown in FIGS. 3, 11 and 18) or with unequal (or asymmetrical) diameter 15 (as shown in FIG. 14). A balloon 10 having outer lumens 11 with equal diameter 15 is well suited for a "standard Rapid Exchange" catheter (shown in FIGS. 3 and 6) or an "over-the-wire" catheter type, each having a guidewire lumen 21 (and/or a guidewire 45) extending through one of the balloon's outer lumens. A balloon 10 having outer lumens 11 with equal diameter 15 is also well suited for a "tip Rapid Exchange" catheter type having only the source wire lumen extending through a treatment channel 50 contained within the balloon central lumen 12 (shown in FIG. 11).

Referring to FIG. 14, fluted outer lumens 11 with unequal diameter 15 would provide the offset necessary to compensate for the slight eccentricity in the location of a treatment channel 50 (with the radiation source wire lumen 22 in it) within the central lumen 12 of the balloon 10. A balloon arrangement having outer lumens 11 with unequal diameters (for example, a balloon assembly with one small "flute" and two large "flutes") is best suited for the "standard RX" or "over-the-wire" catheter

designs where the catheter shaft (or inner member) 41 includes two parallel lumens:
a source lumen 22 (for a radiation source 25) and a guidewire lumen 21 (for a
guidewire 45). For very small diameter centering balloon catheters, such as the 2
mm diameter balloon catheter designs, the small “flute” 11 shown in FIG. 14 may be
5 eliminated to provide for centering of the radiation source lumen 22.

The multi-lumen balloon 10 is manufactured using balloon materials, such as
Pebax™, nylon, polyethylene, polyurethane, or polyester. Materials for use in
fabricating the multi-lumen balloon 10 of the present invention are selected by
considering the properties and characteristics (e.g., softness, durability, low
10 stiffness) required by angioplasty balloons, as well as considering properties
necessary for successful balloon fabrication (e.g., balloon material compatible with
other catheter materials and bonding process, material extruding well, etc.). When
deployed (i.e., inflated), the multi-lumen balloon 10 is a high strength, flexible,
reasonably noncompliant balloon. The fluted shape of the balloon outer lumens
15 allows the balloon to have improved blood perfusion capability as well as improved
balloon refolding characteristics (when the inflation medium is removed from the
balloon outer lumens).

Fluted Balloon Radiation Centering Catheter Assembly

20 With reference to FIGS. 1-16, four types of fluted balloon radiation centering
catheter assemblies are illustrated. In FIGS. 1-5, a fluted balloon radiation
centering catheter assembly 1 for a “standard Rapid Exchange” catheter with a

guidewire lumen 21 extending through one of the outer lumens is shown. In FIGS. 5-9, a fluted balloon radiation centering catheter assembly 1 for a standard Rapid Exchange catheter 2 with proximal and distal slideable seals is shown. In FIGS. 10-12, a fluted balloon radiation centering catheter assembly 1 for a “tip (or distal) Rapid Exchange” catheter 2 is illustrated. Finally, in FIGS. 13-16, a fluted balloon radiation centering catheter assembly 1 for a standard Rapid Exchange catheter 2 with a guidewire lumen 21 extending through the central lumen 12 is shown.

Multi-lumen Balloon Catheter Having a Guidewire Lumen Through Balloon

Outer Lumen

Referring to FIG. 1, a multi-lumen fluted balloon radiation centering catheter assembly 1 with the balloon 10 in an inflated state is shown. The fluted balloon radiation centering catheter assembly 1 includes a multi-lumen balloon 10 and an interventional catheter 2. Interventional catheter 2 has a shaft 41 disposed proximate the balloon 10. The balloon 10 includes a plurality of inflatable outer lumens 11 disposed around a central lumen 12, the plurality of outer lumens 11 integrally coupled with the central lumen 12 so as to form the multi-lumen balloon 10. The balloon 10 has a distal seal 28 and a proximal seal 29. Distal seal 28 seals the plurality of distal ends 34b of the balloon outer lumens 11 to the catheter shaft 41 while the proximal seal 29 seals the plurality of proximal ends 34a of the balloon outer lumens 11 to the catheter shaft 41. Each of the outer lumens 11 takes the form of a “flute” (i.e., an elongated cylinder having tapered ends) when inflated by

an inflation medium 18b (shown in Fig. 3 for this balloon catheter assembly). A fluted balloon configuration is shown in FIG. 17, which is a representative illustration of balloon configurations of this invention (as revealed in balloon catheter assemblies of FIGS. 1, 6, 10, and 13).

5 Referring now to FIG. 3, the multi-lumen balloon catheter assembly 1 has a radiation source lumen 22 that extends longitudinally through the central lumen 12 of the four-lumen balloon 10. In one embodiment, for a “standard Rapid Exchange” (standard RX) or an “over-the-wire” (OTW) catheter type, a guidewire lumen 21 (capable of containing a guidewire 45) extends through one of the balloon outer
10 lumens (as shown in FIG. 3). The guidewire 45 allows positioning the multi-lumen centering catheter 1 (including its radiation source lumen 22) on the stenosed body vessel area 16 for patient treatment.

The balloon radiation centering catheter assembly shown in FIG. 3 may also be used with a “tip (or distal) Rapid Exchange” catheter type, with a guidewire
15 lumen 21 is distally positioned to the multi-lumen balloon 10 and thus would not pass through the balloon 10.

For a “Standard RX” catheter type, the guidewire exists the catheter shaft at a distance in a range of approximately 15-35 cm from the distal tip of the catheter. For a “tip RX” catheter type, the guidewire exists the catheter shaft at a distance in
20 a range of approximately 3-20 mm from the distal tip of the catheter. Note that for a tip RX catheter type, the guidewire does not enter the balloon. For the “OTW” catheter type, the guidewire extends through the catheter shaft. The distance from

the distal tip of the catheter to the inflation port may be in a range of approximately 75-135 cm for coronary applications and in a range of approximately 75-145 cm for peripheral applications. For any catheter type, if an afterloader (i.e., radiation therapy device) is to be used, the guidewire may be extended an additional 15-125
5 cm. In one embodiment, when using the afterloader the guidewire extension may be in a range of approximately 70-80 cm.

Continuing with reference to FIG. 3, as mentioned above, the radiation source lumen 22 extends longitudinally through the balloon central lumen and the standard RX guidewire lumen 21 extends longitudinally through one of the balloon
10 outer lumens 11. The remaining two outer lumens 11 are then sealed onto the radiation source lumen 22 and the guidewire lumen 21 for maintaining inflation pressure in the balloon. When inflated by an inflation medium 18b, the balloon outer lumens 11 form flutes positioned parallel to the radiation source lumen 22 and the guidewire lumen 21. During vascular radiotherapy, when inflated and engaged
15 with the walls of the body vessel 16, the balloon outer lumens 11 define a series of straight longitudinal paths 14 that allow for perfusion of blood (not shown) past balloon treatment area 30 (shown in FIG. 1).

The fluted balloon outer lumens 11 can be extruded with either equal diameter 15 (as shown in FIGS. 3, 11 and 18) or with unequal (or asymmetrical)
20 diameter 15 (as shown in FIG. 14). A balloon 10 having outer lumens 11 with equal diameter 15 is well suited for a "standard Rapid Exchange" catheter (shown in FIGS. 3 and 6) or an "over-the-wire" catheter type, each having a guidewire lumen

21 (and/or a guidewire 45) extending through one of the balloon's outer lumens. A balloon 10 having outer lumens 11 with equal diameter 15 is also well suited for a "tip Rapid Exchange" catheter type having only the source wire lumen extending through a treatment channel 50 contained within the balloon central lumen 12 (shown in FIG. 11).

Continuing with reference to FIG. 3, the diameter 18a of the balloon central lumen 12 is sized based on the radiation source outer diameter, for example a radiation source wire having an outer diameter in a range of approximately 10/1000 in. to 50/1000 in. The combined balloon diameter 13 (as measured across all balloon outer lumens 11 while balloon is in an inflated or deployed state) is kept in a range of approximately 1.5 mm to 6 mm for coronary vessels and in a range of approximately 3 mm to 12 mm for peripheral vessels. For the embodiment shown in FIG. 3, a balloon having a combined diameter 13 in a range of approximately 1.5 mm to 4 mm is advantageous when treating coronary vessels.

Referring to FIG. 4 (which represents a cross-sectional view of the multi-lumen fluted balloon radiation centering catheter assembly of FIG. 1 taken along line C—C), the catheter shaft 41 includes an inner lumen 41a that extends longitudinally through at least a portion of the catheter shaft 41 proximate the balloon 10 and connects to the central lumen 12 of the balloon 10. The catheter shaft inner lumen 41a is adapted for receiving a radiation source lumen 22 with a radiation source 25 and a guidewire lumen 21 capable of containing a guidewire 45 for positioning the multi-lumen balloon radiation centering catheter 1 within a body

vessel. Both the radiation source lumen 22 and the guidewire lumen 21 are manufactured as co-extrusions having an inner layer made of a material such as polyethylene and an outer layer made of a material such as Pebax, nylon, or Primacor.

5 Continuing with reference to FIG. 4, the catheter shaft inner lumen 41a is further adapted to receive at least one inflation lumen (54b, 55b) that is in fluid communication with each of the balloon outer lumens to allow an inflation fluid to enter and inflate the outer lumens 11 and thus, center the radiation source lumen 22 within a body vessel 16. The inflation lumen(s) (54b, 55b) in the catheter shaft inner
10 lumen 41a are generally formed when the multi-lumen balloon 10 is bonded to the catheter shaft 41 during the catheter proximal seal 29 construction (explained in more detail in the Proximal Seal section).

As mentioned above, having individual inflation lumens for each of the balloon outer lumens allows each balloon outer lumen to be inflated to different
15 pressures. However, it is not necessary to have individual inflation lumens for each of the balloon outer lumens in order to center to radiation source lumen with the vessel. For balloon catheter designs where individual inflation lumens (54b, 55b) are absent, the catheter shaft inner lumen 41a may serve as an inflation lumen for the balloon outer lumens 11.

20 Referring to FIG. 5 (which represents a cross-sectional view of the multi-lumen fluted balloon radiation centering catheter assembly of FIG. 1 taken along line D—D), at the region of the balloon catheter proximal seal 29, an elongated

flexible catheter outer member 46 is placed over the catheter shaft 41. The catheter outer member may be manufactured of materials such as nylon, Pebax, polyurethane, etc. Catheter outer member 46 includes a lumen 50a that extends longitudinally therein. Near the catheter proximal seal 29 region, the lumen 50a becomes the catheter shaft inner lumen 41a. Lumen 50a is adapted for receiving a common inflation lumen 36 for inflating and pressurizing the balloon outer lumens 11 with an inflation medium (or means) 18b. The inflation medium 18b could include any inflation medium known in the art of balloon angioplasty, such as air, saline solution, or contrast fluid.

Continuing with reference to FIG. 5, the catheter outer member inner lumen 50a is adapted for receiving a radiation source lumen 22 with a radiation source 25. If a Standard RX (Rapid Exchange) or an OTW interventional catheter assembly 2 is used, the catheter outer member lumen 50a is further adapted for receiving a guidewire lumen 21 (and/or a guidewire 45).

Referring now to FIG. 1, the multi-lumen balloon has a treatment area 30 is defined between the balloon's distal seal 28 and proximal seal 29. The longitudinal length of the balloon treatment area 30 is made to be appropriate for the body vessel to be treated (for example, coronary vessels or peripheral vessels) and for the radiation treatment to be delivered. In one embodiment of the present invention, the balloon treatment area length 30 is in a range of approximately 18 mm to 54 mm. For some intervascular gamma radiation treatments, such as treatments on

peripheral vessels of the cardiovascular system, the balloon treatment area length 30 may be in a range of approximately 10 mm to 250 mm.

Continuing with reference to FIG. 1, in one embodiment, the radiation source lumen 22 is sealed at its distal end 23 with plug 24 to allow a radiation source 25 to
5 be placed inside the radiation source lumen 22. In another embodiment, the radiation source lumen 22 is left open at its distal end 23 (i.e., it does not have a plug 24) so that a radiation source 25 (placed inside the radiation source lumen 22) can be distally advanced past the multi-lumen balloon 10. Furthermore, not having the radiation source lumen 22 sealed with the plug 24 decreases the stiffness of the
10 multi-lumen balloon even further.

It should be noted that it is not necessary to have a radiation source lumen 22 as part of the multi-lumen balloon centering catheter assembly 1. In some applications, it may be desirable to place the radiation source 25 directly within the central lumen 12 of the balloon 10, without employing a source lumen 22. Not
15 having a radiation source lumen 22 in the balloon central lumen 12 reduces the size of the multi-lumen balloon and decreases the stiffness of the multi-lumen balloon (since the radiation source lumen 22 is a co-extruded shaft), thus allowing the balloon to cross tortuous paths more easily along the body vessel.

The radiation source 25, which may be shaped in the form of a wire, seed,
20 pellets, ribbon, etc., is positioned inside radiation source lumen 22 and is then advanced longitudinally along a prescribed vessel length 16 during patient treatment. In one embodiment of this invention, the multi-lumen balloon centering

catheter assembly 1 uses a Phosphorus-32 radiation source as a radiation source 24. However, the multi-lumen balloon of this invention can be used with any radiation source employed in vascular radiotherapy, which includes gamma radiation emitting sources and beta radiation emitting sources known in the art.

5 Continuing with reference to FIG. 1, two radio-opaque markers, a distal marker 37 and a proximal marker 38, may be attached to the radiation source lumen 22. The radio-opaque markers 37 and 38 are used for positioning the interventional catheter 1 under fluoroscopy, as well as for assisting the stepping (via manual or automatic means) of the radiation source 25 over the entire prescribed 10 region of the vessel 16 to be treated. The markers 37 and 38 are made of any materials known in the art of radio-opaque markers, such as silver, gold, platinum, tungsten, that allow markers to become visible under fluoroscopy. In one embodiment, the radio-opaque markers (37, 38) are attached within the limits of the balloon's treatment area 30. In one configuration, the distal marker 37 is 15 incorporated into the plug 24 of the source lumen 22. In another configuration, radio-opaque markers (37, 38) may be part of a separate device (not shown) that is independent of the balloon catheter assembly.

A soft tip 26 is attached to the distal end 27 of the guidewire lumen 21 to improve trackability and reduce trauma to the body vessel. The length of the soft tip 20 26 depends on the type of catheter design used, however, the length of the tip is generally in a range of approximately 0.5 mm to 10 mm.

With reference to FIG. 1, the balloon 10 is attached to catheter shaft 41 of the catheter assembly 2. The balloon's proximal seal 29 is attached at a proximal end 44 of flexible catheter shaft 41, near the inflation/deflation port 33. The balloon distal seal 28 is attached to the catheter shaft 41 adjacent to the location where the radiation source lumen 22 ends. In one embodiment, the balloon 10 and assembly 2 are attached by using a laser bond technique. Bonds may also be done using other balloon bonding techniques known in the art, such as thermal or ultrasonic welds, adhesive welds, or other conventional means. The distal and proximal seals (28, 29) may each have a width in a range of approximately 0.5 mm to about 5 mm.

Multi-lumen Balloon Catheter Having a Slideable Proximal Seal and a Slideable Distal Seal

Referring to FIGS. 6-9, a fluted balloon radiation centering catheter assembly for a standard Rapid Exchange catheter with proximal and distal slideable seals is shown. In the embodiment disclosed herein, the tubing used to form the guidewire lumen is eliminated, and is replaced by proximal slideable seal 29a and distal slideable seal 28a as shown in FIG 6. Eliminating the guidewire tubing reduces the material used and lowers the balloon catheter proximal seal outer diameter. These improvements make the catheter less stiff, allowing the balloon catheter to cross tortuous paths more easily along the body vessel. Furthermore, eliminating the guidewire tubing allows the proximal seal to become less complicated during seal manufacturing (as discussed in more detail in a later section).

With reference to FIG. 6, the path of the rapid exchange guidewire 45 starts at the distal tip 26 of the catheter 1 by entering an annular space 45b (shown in FIG. 7) formed between the catheter shaft 41 and the distal end of the radiation source lumen 22. This is where the slideable distal seal 28a is located. The guidewire 45 then longitudinally passes through one of the balloon outer lumens 11, where the balloon outer lumen 11 itself acts as a guidewire lumen. The guidewire 45 then runs in the annular space 52 (shown in FIG. 8) between the shaft outer member 46 and the source lumen 22 until it reaches an exit notch 29b with a slideable proximal seal 29a. These annular spaces 45b and 52 are also used to inflate and deflate the multi-lumen balloon, so “slideable” seals are used at both the catheter tip 26 and at the guidewire exit notch 29b.

Referring to FIG. 7, as stated above, the guidewire 45 enters an annular space 45b (shown in FIG. 7) formed between the catheter shaft 41 and the distal end of the radiation source lumen 22. To create the slideable distal seal 28a, the annular space 45b is made to be a “close fit” by having a minimal distance clearance between the outer diameter of the guidewire 45 and the inner diameter of the balloon seal (formed when the balloon is being bonded to the catheter shaft).

Referring to FIG. 8, after exiting the balloon outer lumen, the guidewire 45 then enters an annular space 52 (shown in FIG. 8) formed in the catheter shaft outer member 46. The annular space (or lumen) 52 serves both as a lumen for the guidewire 45 and as an inflation lumen for the balloon outer lumen that has the guidewire contained therein.

The slideable distal and proximal seals (28a, 29a) prevent the balloon inflation media (for example, saline) (not shown) from leaking out of the catheter 2. However, the slideable seals (28a, 29a) to the guidewire 45 are not fixed, rather the design allows the guidewire to slide axially relative to the catheter 2 and also allows the guidewire 45 to be rotated relative to the catheter. In one embodiment, the combination of a sealing capability with relative motion is obtained by having minimal clearances between the outer diameter of the guidewire 45 and the inner diameter 45aa of the seal formed between the balloon and the catheter shaft (as shown in FIG. 7).

Another embodiment of the slideable proximal and distal seals uses a hydrogel material 45a (shown in FIG. 7), positioned either on the guidewire 45 or integral to the slideable distal and proximal seals (28a, 29a) to maintain the pressure seal while providing smoother movement of the guidewire 45. To insure that the seals (28a, 29a) hold pressure, the catheter 2 may be used with guidewires that have a polymer jacket rather than an intermediate wire coil. In a yet another embodiment, the hydrogel material in the slideable proximal and distal seals is substituted with an O-ring 45a (shown in FIG. 9). This O-ring is positioned either on the guidewire 45 or integral to the slideable distal and proximal seals (28a, 29a) to maintain the pressure seal while providing smoother movement of the guidewire 45.

Referring to FIG. 6, a multi-lumen fluted balloon radiation centering catheter assembly 1 with the balloon 10 in an inflated state is shown. The fluted balloon radiation centering catheter assembly 1 includes a multi-lumen balloon 10 and an

interventional catheter 2. Interventional catheter 2 has a shaft 41 disposed proximate to the balloon 10. The balloon 10 includes a plurality of inflatable outer lumens 11 disposed around a central lumen 12, the plurality of outer lumens 11 integrally coupled with the central lumen 12 so as to form the multi-lumen balloon 10. The balloon 10 has a slideable distal seal 28a and a slideable proximal seal 29a. Slideable distal seal 28a seals the plurality of distal ends 34b of the balloon outer lumens 11 to the catheter shaft 41 while the slideable proximal seal 29a seals the plurality of proximal ends 34a of the balloon outer lumens 11 to the catheter shaft 41.

Each of the outer lumens 11 takes the form of a “flute” (i.e., an elongated cylinder having tapered ends) when inflated by an inflation medium. A fluted balloon configuration is shown in FIG. 17, which is a representative illustration of balloon configurations of this invention. During vascular radiotherapy, when inflated and engaged with the walls of the body vessel 16, the balloon outer lumens 11 define a series of straight longitudinal paths that allow for perfusion of blood past a balloon treatment area 30 (shown in FIG. 6). The longitudinal length of the balloon treatment area 30 is made to be appropriate for the body vessel to be treated (for example, coronary vessels or peripheral vessels) and for the radiation treatment to be delivered. In one embodiment of the present invention, the balloon treatment area length 30 is in a range of approximately 18 mm to 54 mm. For some intervascular gamma radiation treatments, such as treatments on peripheral vessels

of the cardiovascular system, the balloon treatment area length 30 may be in a range of approximately 10 mm to 250 mm.

The fluted balloon outer lumens 11 can be extruded with either equal diameter 15 (as shown in FIGS. 3, 11 and 18) or with unequal (or asymmetrical) diameter 15 (as shown in FIG. 14).

Continuing with reference to FIG. 6, the balloon central lumen 12 is sized based on the radiation source outer diameter, for example a radiation source wire having an outer diameter in a range of approximately 10/1000 in. to 50/1000 in. The combined balloon diameter 13 (as measured across all balloon outer lumens 11 while balloon is in an inflated or deployed state) is kept in a range of approximately 1.5 mm to 6 mm for coronary vessels and in a range of approximately 3 mm to 12 mm for peripheral vessels. For the embodiment shown in FIG. 6, a balloon having a combined diameter 13 in a range of approximately 1.5 mm to 4 mm is advantageous when treating coronary vessels.

Continuing with reference to FIG. 6, the multi-lumen balloon catheter assembly 1 has a radiation source lumen 22 that extends longitudinally through the central lumen 12 of the four-lumen balloon 10. In this embodiment, a guidewire 45 without a guidewire lumen tubing extends through one of the balloon outer lumens (as shown in FIG. 6). The guidewire 45 allows positioning the multi-lumen centering catheter 1 (including its radiation source lumen 22) on the stenosed body vessel area for patient treatment.

Continuing with reference to FIG. 6, in one embodiment, the radiation source lumen 22 is sealed at its distal end with plug 24 to allow a radiation source 25 to be placed inside the radiation source lumen 22. In another embodiment, the radiation source lumen 22 is left open at its distal end 23 (i.e., it does not have a plug 24) so that a radiation source 25 (placed inside the radiation source lumen 22) can be distally advanced past the multi-lumen balloon 10. Furthermore, not having the radiation source lumen 22 sealed with the plug 24 decreases the stiffness of the multi-lumen balloon even further.

It should be noted that it is not necessary to have a radiation source lumen 22 as part of the multi-lumen balloon centering catheter assembly 1. In some applications, it may be desirable to place the radiation source 25 directly within the central lumen 12 of the balloon 10, without employing a source lumen 22. Not having a radiation source lumen 22 in the balloon central lumen 12 reduces the size of the multi-lumen balloon and decreases the stiffness of the multi-lumen balloon (since the radiation source lumen 22 is a co-extruded shaft), thus allowing the balloon to cross tortuous paths more easily along the body vessel.

The radiation source 25, which may be shaped in the form of a wire, seed, pellets, ribbon, etc., is positioned inside radiation source lumen 22 and is then advanced longitudinally along a prescribed vessel length 16 during patient treatment. In one embodiment of this invention, the multi-lumen balloon centering catheter assembly 1 uses a Phosphorus-32 radiation source as a radiation source 24. However, the multi-lumen balloon of this invention can be used with any

radiation source employed in vascular radiotherapy, which includes gamma radiation emitting sources and beta radiation emitting sources known in the art.

Continuing with reference to FIG. 6, two radio-opaque markers, a distal marker 37 and a proximal marker 38, may be attached to the radiation source lumen 22. The radio-opaque markers 37 and 38 are used for positioning the interventional catheter 1 under fluoroscopy, as well as for assisting the stepping (via manual or automatic means) of the radiation source 25 over the entire prescribed region of the vessel 16 to be treated. The markers 37 and 38 are made of any materials known in the art of radio-opaque markers, such as silver, gold, platinum, tungsten, that allow markers to become visible under fluoroscopy. In one embodiment, the radio-opaque markers (37, 38) are attached within the limits of the balloon's treatment area 30. In one configuration, the distal marker 37 is incorporated into the plug 24 of the source lumen 22. In another configuration, radio-opaque markers (37, 38) may be part of a separate device (not shown) that is independent of the balloon catheter assembly.

A soft tip 26 (shown in FIG. 6) is attached to the distal end 27 of the guidewire 45 to improve trackability and reduce trauma to the body vessel. The length of the soft tip 26 depends on the type of catheter design used, however, the length of the tip is generally in a range of approximately 0.5 mm to 10 mm.

Referring now to FIG. 8 (which represents a cross-sectional view of the multi-lumen fluted balloon radiation centering catheter assembly of FIG. 6 taken along line F—F), the catheter shaft 41 includes an inner lumen 41a that extends

longitudinally through at least a portion of the catheter shaft 41 proximate the balloon 10 and connects to the central lumen 12 of the balloon 10. The catheter shaft inner lumen 41a is adapted for receiving a radiation source lumen 22 with a radiation source 25. The radiation source lumen 22 is manufactured as a co-extruded shaft having an inner layer made of a material such as polyethylene and an outer layer made of a material such as Pebax, nylon, or Primacor.

Continuing with reference to FIG. 8, the catheter shaft inner lumen 41a is further adapted to receive a plurality of inflation lumens (51, 52) that are in fluid communication with each of the balloon outer lumens to allow an inflation fluid to enter and inflate the outer lumens 11 and thus, center the radiation source lumen 22 within a body vessel 16. Note that lumen 52 serves as both an inflation lumen and as a guidewire lumen. The inflation lumens (51, 52) in the catheter shaft inner lumen 41a are generally formed when the multi-lumen balloon 10 is bonded to the catheter shaft 41 during the catheter slideable proximal seal 29a construction. As mentioned above, having individual inflation lumens for each of the balloon outer lumens allows each balloon outer lumen to be inflated to different pressures.

Referring to FIG. 9 (which represents a cross-sectional view of the multi-lumen fluted balloon radiation centering catheter assembly of FIG. 6 taken along line G—G), at the region of the balloon catheter slideable proximal seal 29a, an elongated flexible catheter outer member 46 is placed over the catheter shaft 41. Catheter outer member 46 includes a lumen 50a that extends longitudinally therein.

Past the catheter slideable proximal seal 29a region, the lumen 50a becomes the catheter shaft inner lumen 41a.

Lumen 50a is adapted for receiving a common inflation lumen 36 for inflating and pressurizing the balloon outer lumens 11 with an inflation medium (or means) 18b. The inflation medium 18b could include any inflation medium known in the art of balloon angioplasty, such as air, saline solution, or contrast fluid. The catheter outer member inner lumen 50a is further adapted for receiving a radiation source lumen 22 (with a radiation source) and a guidewire lumen 21. At the slideable proximal seal 29a, to ensure a tight and close fit, the guidewire lumen 21 in the catheter outer member 46 is adapted for receiving a hydrogel material or an O-ring 45a. The catheter outer member 46 may be manufactured of materials such as nylon, Pebax, polyurethane, etc.

Multi-lumen Balloon Catheter Having a Balloon with Communication Bores between Central and Outer Lumens and a Tip Rapid Exchange Guidewire Lumen

With reference to FIGS. 10-16, two embodiments of a multi-lumen fluted balloon radiation centering catheter assembly are shown. Both catheter assemblies include a multi-lumen balloon having communication bores between the central lumen and the outer lumens. In FIGS. 10-12, a fluted balloon radiation centering catheter assembly for a "tip (or distal) Rapid Exchange" catheter 2 is illustrated, while in FIGS. 13-16, a fluted balloon radiation centering catheter assembly 1 for a standard Rapid Exchange catheter with a guidewire lumen extending through the central lumen is shown.

Referring to FIG. 10, a multi-lumen fluted balloon radiation centering catheter assembly 1 with the balloon 10 in an inflated state is shown. The fluted balloon radiation centering catheter assembly 1 includes a multi-lumen balloon 10 and an interventional catheter 2. Interventional catheter 2 has a shaft disposed proximate the balloon 10. The balloon 10 includes a plurality of inflatable outer lumens 11 disposed around a central lumen 12, the plurality of outer lumens 11 integrally coupled with the central lumen 12 so as to form the multi-lumen balloon 10. The balloon 10 has a distal seal 28 and a proximal seal 29. Distal seal 28 seals the plurality of distal ends 34b of the balloon outer lumens 11 to the catheter shaft 41 while the proximal seal 29 seals the plurality of proximal ends 34a of the balloon outer lumens 11 to the catheter shaft 41. The distal and proximal seals (28, 29) may each have a width in a range of approximately 0.5 mm to about 5 mm.

Each of the outer lumens 11 takes the form of a “flute” (i.e., an elongated cylinder having tapered ends) when inflated by an inflation medium 18b (shown in Fig. 11 for this balloon catheter assembly). A fluted balloon configuration is shown in FIG. 17, which is a representative illustration of balloon configurations of this invention (as revealed in balloon catheter assemblies of FIGS. 1, 6, 10, and 13).

Continuing with reference to FIG. 10, the catheter shaft includes an inner tubular member 41 having a distal treatment section 42 with a distal end 43 and a proximal end 44, and a proximate section (not shown). The inner tubular member 41 has an inner lumen 41a. The catheter shaft further includes a flexible elongate outer tubular member 46 having a distal section 47 with a distal end 48, and a

proximate section (not shown). Elongate inner tubular member 41 extends coaxially within the elongate outer tubular member 46.

Referring now to FIG. 11, the balloon central lumen 12 is capable of containing a radiation source 25 (with or without a radiation source lumen 22) therein. The multi-lumen balloon embodiment shown in FIG 11 is adapted for receiving a guidewire lumen (with a guidewire) through its central lumen 12 (as shown in FIG 14). Because in FIG. 11 the balloon 10 is shown as being used with a tip (or distal) Rapid Exchange catheter type (i.e., the guidewire is positioned distal to the balloon), for the balloon embodiment of FIG. 11, the guidewire does not extend through any of the balloon lumens 11.

For the balloon configuration shown in FIG. 11, the balloon 10 includes bores (or channels) 35 that are formed between the outer lumens 11 and the central lumen 12. This arrangement allows an inflation medium 18b to pass from the balloon central lumen 12 into the outer lumens 11 and inflate outer lumens 11, causing a radiation source lumen 22 to be centered within a body vessel 16. In this configuration, the central lumen 12 is pressurized in order for the outer lumens 11 to properly inflate and center the radiation source lumen 22 within the body vessel 16. The catheter inner lumen 41a is adapted to serve as an inflation lumen for the balloon central lumen 12 and the outer lumens 11.

Continuing with reference to FIG. 11, as mentioned above, the radiation source lumen 22 extends longitudinally through the balloon central lumen. When using a tip RX radiation catheter type, the plurality of outer lumens 11 are sealed

onto the radiation source lumen 22 for maintaining inflation pressure in the balloon. When inflated by an inflation medium 18b, the balloon outer lumens 11 form flutes positioned parallel to the radiation source lumen 22. During vascular radiotherapy, when inflated and engaged with the walls of the body vessel 16, the balloon outer lumens 11 define a series of straight longitudinal paths 14 that allow for perfusion of blood (not shown) past balloon treatment area 30 (shown in FIG. 10).

The fluted balloon outer lumens 11 can be extruded with either equal diameter 15 (as shown in FIG. 11) or with unequal (or asymmetrical) diameter 15 (as shown in FIG. 14). A balloon 10 having outer lumens 11 with equal diameter 15 is well suited for a "tip Rapid Exchange" catheter type having only the source wire lumen extending through a treatment channel 50 contained within the balloon central lumen 12 (shown in FIG. 11).

Continuing with reference to FIG. 11, the diameter 18a of the balloon central lumen 12 is sized based on the radiation source outer diameter, for example a radiation source wire having an outer diameter in a range of approximately 10/1000 in. to 50/1000 in. The combined balloon diameter 13 (as measured across all balloon outer lumens 11 while balloon is in an inflated or deployed state) is kept in a range of approximately 1.5 mm to 6 mm for coronary vessels and in a range of approximately 3 mm to 12 mm for peripheral vessels. For the embodiment shown in FIG. 11, a balloon having a combined diameter 13 in a range of approximately 1.5 mm to 4 mm is advantageous when treating coronary vessels.

Referring now to FIG. 10, the multi-lumen balloon has a treatment area 30 is defined between the balloon's distal seal 28 and proximal seal 29. The longitudinal length of the balloon treatment area 30 is made to be appropriate for the body vessel to be treated (for example, coronary vessels or peripheral vessels) and for the radiation treatment to be delivered. In one embodiment of the present invention, the balloon treatment area length 30 is in a range of approximately 18 mm to 54 mm. For some intervascular gamma radiation treatments, such as treatments on peripheral vessels of the cardiovascular system, the balloon treatment area length 30 may be in a range of approximately 10 mm to 250 mm.

Continuing with reference to FIG. 10, in one embodiment, the radiation source lumen 22 is sealed at its distal end 23 with plug 24 to allow a radiation source 25 to be placed inside the radiation source lumen 22. In another embodiment, the radiation source lumen 22 is left open at its distal end 23 (i.e., it does not have a plug 24) so that a radiation source 25 (placed inside the radiation source lumen 22) can be distally advanced past the multi-lumen balloon 10. Furthermore, not having the radiation source lumen 22 sealed with the plug 24 decreases the stiffness of the multi-lumen balloon even further.

It should be noted that it is not necessary to have a radiation source lumen 22 as part of the multi-lumen balloon centering catheter assembly 1. In some applications, it may be desirable to place the radiation source 25 directly within the central lumen 12 of the balloon 10, without employing a source lumen 22. Not having a radiation source lumen 22 in the balloon central lumen 12 reduces the size

of the multi-lumen balloon and decreases the stiffness of the multi-lumen balloon (since the radiation source lumen 22 is a co-extruded shaft), thus allowing the balloon to cross tortuous paths more easily along the body vessel.

The radiation source 25, which may be shaped in the form of a wire, seed, pellets, ribbon, etc., is positioned inside radiation source lumen 22 and is then advanced longitudinally along a prescribed vessel length 16 during patient treatment. In one embodiment of this invention, the multi-lumen balloon centering catheter assembly 1 uses a Phosphorus-32 radiation source as a radiation source 24. However, the multi-lumen balloon of this invention can be used with any radiation source employed in vascular radiotherapy, which includes gamma radiation emitting sources and beta radiation emitting sources known in the art.

Continuing with reference to FIG. 10, two radio-opaque markers, a distal marker 37 and a proximal marker 38, may be attached to the radiation source lumen 22. The radio-opaque markers 37 and 38 are used for positioning the interventional catheter 1 under fluoroscopy, as well as for assisting the stepping (via manual or automatic means) of the radiation source 25 over the entire prescribed region of the vessel 16 to be treated. The markers 37 and 38 are made of any materials known in the art of radio-opaque markers, such as silver, gold, platinum, tungsten, that allow markers to become visible under fluoroscopy. In one embodiment, the radio-opaque markers (37, 38) are attached within the limits of the balloon's treatment area 30. In one configuration, the distal marker 37 is incorporated into the plug 24 of the source lumen 22. In another configuration,

radio-opaque markers (37, 38) may be part of a separate device (not shown) that is independent of the balloon catheter assembly.

A soft tip 26 is attached to the distal end 27 of the guidewire lumen 21 to improve trackability and reduce trauma to the body vessel. The length of the soft tip 26 depends on the type of catheter design used, however, the length of the tip is generally in a range of approximately 0.5 mm to 10 mm.

With reference to FIG. 10, the balloon 10 is attached to catheter shaft 41 of the catheter assembly 2. The balloon's proximal seal 29 is attached at a proximal end 44 of flexible catheter shaft 41, near the inflation/deflation port 33. The balloon distal seal 28 is attached to the catheter shaft 41 adjacent to the location where the radiation source lumen 22 ends. In one embodiment, the balloon 10 and assembly 2 are attached by using a laser bond technique. Bonds may also be done using other balloon bonding techniques known in the art, such as thermal or ultrasonic welds, adhesive welds, or other conventional means.

Multi-lumen Balloon Catheter Having a Balloon with Communication Bores between Central and Outer Lumens and a Guidewire Lumen Through the Central Lumen

In FIGS. 13-16, a fluted balloon radiation centering catheter assembly 1 for a standard Rapid Exchange catheter with a guidewire lumen extending through the central lumen of a multi-lumen balloon is shown.

Referring to FIG. 13, a multi-lumen fluted balloon radiation centering catheter assembly 1 with the balloon 10 in an inflated state is shown. The fluted balloon radiation centering catheter assembly 1 includes a multi-lumen balloon 10 and an interventional catheter 2. Interventional catheter 2 has a shaft disposed proximate the balloon 10. The balloon 10 includes a plurality of inflatable outer lumens 11 disposed around a central lumen 12, the plurality of outer lumens 11 integrally coupled with the central lumen 12 so as to form the multi-lumen balloon 10. The balloon 10 has a distal seal 28 and a proximal seal 29. Distal seal 28 seals the plurality of distal ends 34b of the balloon outer lumens 11 to the catheter shaft 41 while the proximal seal 29 seals the plurality of proximal ends 34a of the balloon outer lumens 11 to the catheter shaft 41. The distal and proximal seals (28, 29) may each have a width in a range of approximately 0.5 mm to about 5 mm.

Each of the outer lumens 11 takes the form of a "flute" (i.e., an elongated cylinder having tapered ends) when inflated by an inflation medium 18b (shown in Fig. 14 for this balloon catheter assembly). A fluted balloon configuration is shown in FIG. 17, which is a representative illustration of balloon configurations of this invention (as revealed in balloon catheter assemblies of FIGS. 1, 6, 10, and 13).

Continuing with reference to FIG. 13, the catheter shaft includes an inner tubular member 41 having an inner lumen 41a. The catheter shaft further includes a flexible elongate outer tubular member 46. Elongate inner tubular member 41 extends coaxially within the elongate outer tubular member 46.

Referring now to FIG. 14, the balloon central lumen 12 is capable of containing a radiation source 25 (with or without a radiation source lumen 22) therein. The multi-lumen balloon embodiment shown in FIG 14 is further adapted for receiving a guidewire lumen (with a guidewire 45) through its central lumen 12.

5 For the balloon configuration shown in FIG. 14, the balloon 10 includes bores (or channels) 35 that are formed between the outer lumens 11 and the central lumen 12. This arrangement allows an inflation medium 18b to pass from the balloon central lumen 12 into the outer lumens 11 and inflate outer lumens 11, causing a radiation source lumen 22 to be centered within a body vessel 16. In this
10 configuration the central lumen 12 is pressurized in order for the outer lumens 11 to properly inflate and center the radiation source lumen 22 within the body vessel 16. The catheter inner lumen 41a is adapted to serve as an inflation lumen for the balloon central lumen 12 and the outer lumens 11 (as shown in FIG. 16).

Continuing with reference to FIG. 14, when using a standard RX or an over-
15 the-wire radiation catheter type, the radiation source lumen 22 and the guidewire lumen 21 extend longitudinally through the balloon central lumen. The plurality of outer lumens 11 are sealed onto the radiation source lumen 22 and the guidewire lumen 21 for maintaining inflation pressure in the balloon. When inflated by an inflation medium 18b, the balloon outer lumens 11 form flutes positioned parallel to
20 the radiation source lumen 22. During vascular radiotherapy, when inflated and engaged with the walls of the body vessel 16, the balloon outer lumens 11 define a

series of straight longitudinal paths 14 that allow for perfusion of blood (not shown) past balloon treatment area 30 (shown in FIG. 13).

The fluted balloon outer lumens 11 can be extruded with either equal diameter 15 (as shown in FIG. 11) or with unequal (or asymmetrical) diameter 15 (as shown in FIG. 14). A balloon arrangement having outer lumens 11 with unequal diameters (for example, a balloon assembly of FIG. 14 with one small “flute” and two large “flutes”) is best suited for the “standard RX” or “over-the-wire” catheter designs where the catheter shaft (or inner member) 41 includes two parallel lumens: a source lumen 22 (for a radiation source 25) and a guidewire lumen 21 (for a guidewire 45). For very small diameter centering balloon catheters, such as the 2 mm diameter balloon catheter designs, the small “flute” 11 shown in FIG. 14 may be eliminated to provide for centering of the radiation source lumen 22.

Continuing with reference to FIG. 14, the diameter 18a of the balloon central lumen 12 is sized based on the radiation source outer diameter and the guidewire lumen outer diameter, for example a radiation source wire having an outer diameter in a range of approximately 10/1000 in. to 50/1000 in and a guidewire lumen having an outer diameter in a range of approximately 10/1000 in. to 15/1000. The combined balloon diameter 13 (as measured across all balloon outer lumens 11 while balloon is in an inflated or deployed state) is kept in a range of approximately 1.5 mm to 6 mm for coronary vessels and in a range of approximately 3 mm to 12 mm for peripheral vessels. For the embodiment shown in FIG. 14, a balloon having

009700-18090900
a combined diameter 13 in a range of approximately 1.5 mm to 4 mm is advantageous when treating coronary vessels.

Referring now to FIG. 13, the multi-lumen balloon has a treatment area 30 is defined between the balloon's distal seal 28 and proximal seal 29. The longitudinal
5 length of the balloon treatment area 30 is made to be appropriate for the body vessel to be treated (for example, coronary vessels or peripheral vessels) and for the radiation treatment to be delivered. In one embodiment of the present invention, the balloon treatment area length 30 is in a range of approximately 18 mm to 54 mm. For some intervascular gamma radiation treatments, such as treatments on
10 peripheral vessels of the cardiovascular system, the balloon treatment area length 30 may be in a range of approximately 10 mm to 250 mm.

Continuing with reference to FIG. 13, in one embodiment, the radiation source lumen 22 is sealed at its distal end 23 with plug 24 to allow a radiation source 25 to be placed inside the radiation source lumen 22. In another
15 embodiment, the radiation source lumen 22 is left open at its distal end 23 (i.e., it does not have a plug 24) so that a radiation source 25 (placed inside the radiation source lumen 22) can be distally advanced past the multi-lumen balloon 10. Furthermore, not having the radiation source lumen 22 sealed with the plug 24 decreases the stiffness of the multi-lumen balloon even further.

20 It should be noted that it is not necessary to have a radiation source lumen 22 as part of the multi-lumen balloon centering catheter assembly 1. In some applications, it may be desirable to place the radiation source 25 directly within the

central lumen 12 of the balloon 10, without employing a source lumen 22. Not having a radiation source lumen 22 in the balloon central lumen 12 reduces the size of the multi-lumen balloon and decreases the stiffness of the multi-lumen balloon (since the radiation source lumen 22 is a co-extruded shaft), thus allowing the
5 balloon to cross tortuous paths more easily along the body vessel.

The radiation source 25, which may be shaped in the form of a wire, seed, pellets, ribbon, etc., is positioned inside radiation source lumen 22 and is then advanced longitudinally along a prescribed vessel length 16 during patient treatment. In one embodiment of this invention, the multi-lumen balloon centering
10 catheter assembly 1 uses a Phosphorus-32 radiation source as a radiation source 24. However, the multi-lumen balloon of this invention can be used with any radiation source employed in vascular radiotherapy, which includes gamma radiation emitting sources and beta radiation emitting sources known in the art.

Continuing with reference to FIG. 13, two radio-opaque markers, a distal
15 marker 37 and a proximal marker 38, may be attached to the radiation source lumen 22. The radio-opaque markers 37 and 38 are used for positioning the interventional catheter 1 under fluoroscopy, as well as for assisting the stepping (via manual or automatic means) of the radiation source 25 over the entire prescribed region of the vessel 16 to be treated. The markers 37 and 38 are made of any
20 materials known in the art of radio-opaque markers, such as silver, gold, platinum, tungsten, that allow markers to become visible under fluoroscopy. In one embodiment, the radio-opaque markers (37, 38) are attached within the limits of the

balloon's treatment area 30. In one configuration, the distal marker 37 is incorporated into the plug 24 of the source lumen 22. In another configuration, radio-opaque markers (37, 38) may be part of a separate device (not shown) that is independent of the balloon catheter assembly.

5 A soft tip 26 is attached to the distal end of the guidewire lumen 21 to improve trackability and reduce trauma to the body vessel. The length of the soft tip 26 depends on the type of catheter design used, however, the length of the tip is generally in a range of approximately 0.5 mm to 10 mm.

10 With reference to FIG. 13, the balloon 10 is attached to catheter shaft 41 of the catheter assembly 2. The balloon proximal seal 29 is positioned at a proximal end 44 of flexible catheter shaft 41, near the inflation/deflation port 33. The balloon distal seal 28 is positioned to the catheter shaft 41 adjacent to the location where the radiation source lumen 22 ends. In one embodiment, the balloon 10 and assembly 2 are coupled using a laser bond technique. Bonds may also be done
15 using other balloon bonding techniques known in the art, such as thermal or ultrasonic welds, adhesive welds, or other conventional means.

Multi-lumen Balloon Catheter Having a Balloon with or without
Communication Bores between Central and Outer Lumens and A Guidewire
20 Longitudinally Extending Outside the Fluted Balloon Lumens

In FIGS. 27a-27d, a fluted balloon radiation centering catheter assembly 1 for a catheter with a guidewire longitudinally extending outside the multi-lumen balloon is shown.

Referring to FIG. 27a, a multi-lumen fluted balloon radiation centering catheter assembly 1 with the balloon 10 in an inflated state is shown. The fluted balloon radiation centering catheter assembly 1 includes a multi-lumen balloon 10 and an interventional catheter 2. Interventional catheter 2 has a shaft disposed proximate the balloon 10. The balloon 10 includes a plurality of inflatable outer lumens 11 disposed around a central lumen 12, the plurality of outer lumens 11 integrally coupled with the central lumen 12 so as to form the multi-lumen balloon 10. The balloon 10 has a distal seal 28 and a proximal seal 29. Distal seal 28 seals the plurality of distal ends 34b of the balloon outer lumens 11 to the catheter shaft 41 while the proximal seal 29 seals the plurality of proximal ends 34a of the balloon outer lumens 11 to the catheter shaft 41. The distal and proximal seals (28, 29) may each have a width in a range of approximately 0.5 mm to about 5 mm.

Each of the outer lumens 11 takes the form of a "flute" (i.e., an elongated cylinder having tapered ends) when inflated by an inflation medium 18b (shown in Fig. 14 for this balloon catheter assembly). A fluted balloon configuration is shown in FIG. 17, which is a representative illustration of balloon configurations of this invention (as revealed in balloon catheter assemblies of FIGS. 1, 6, 10, 13 and 27a).

Continuing with reference to FIG. 27a, the catheter shaft includes an inner tubular member 41 having an inner lumen 41a (shown in FIG 27b). The catheter shaft 41 further includes a flexible elongate outer tubular member 46. Elongate inner tubular member 41 extends coaxially within the elongate outer tubular member 46.

Still referring to FIG. 27a, two additional guidewire exits (45b1 and 45b2) are notched (or cut out) along the catheter shaft (which includes the tubular member 41) to permit a guidewire 45 to extend lengthwise outside the multi-lumen balloon 10 (see FIG. 27b) from an existing guidewire exit notch 45b3 to a guidewire exit notch 45b2. At the point of the guidewire exit notch 45b2, the guidewire 45 enters the catheter shaft' tubular member 41, extends lengthwise through a portion of the shaft and then exits the shaft at the second guidewire exit notch 45b1. The profile of the fluted balloon with standard RX configuration is 50/1000 in. by 60/1000 in., while the profile of the fluted balloon without the guidewire lumen is about 51/1000 in.

Through this balloon catheter embodiment, the guidewire riding length is extended over the "tip RX" design. This design arrangement has a number of benefits over prior art designs, including (a) maintaining the multi-lumen balloon profile for the "standard RX" design, (b) reducing the profile of the balloon proximal seal, (c) allowing the bore communication between the central lumen and the plurality of outer lumens for an improved centering of the radiation source, and (d) reduces radial shielding effect.

Balloon Treatment Area Markers

As described and shown in figures above, the multi-lumen balloon catheters of this invention may include radio-opaque markers for positioning the interventional catheter 1 under fluoroscopy, as well as for assisting the stepping (via manual or automatic means) of the radiation source 25 over the entire prescribed region of the vessel 16 to be treated. Generally, the markers include a distal marker 37 and a proximal marker 38. Markers 37 and 38 may be attached to the radiation source lumen 22 by adhesive bonding. Markers may also be swaged onto the radiation source lumen.

In yet another embodiment, markers 37 and 38 may be attached directly onto the fluted balloon using a sputtering or vapor deposition process. In this process, a marker material such as gold is deposited onto the balloon using any sputtering or vapor deposition techniques known in the field. It should be noted that the marker material deposition is not limited to a specific area of the multi-lumen balloon; the marker material may be deposited onto the central lumen of the balloon, around the entire circumference of the multi-lumen balloon, or any other balloon area desired.

The markers 37 and 38 may be made of any materials known in the art of radio-opaque markers, such as silver, gold, platinum, tungsten, that allow markers to become visible under fluoroscopy. In one embodiment, the radio-opaque markers (37, 38) are attached within the limits of the balloon's treatment area 30.

Balloon Proximal Seal

A unique proximal seal geometry used to seal a multi-lumen fluted balloon to a catheter shaft and method for manufacturing same is described. In one embodiment (described herein), the proximal seal geometry is used to seal a four-lumen fluted balloon to a shaft containing both a radiation source lumen and a guidewire lumen. In another embodiment (not shown), where the radiation source is used without a radiation source lumen, the proximal seal geometry is used to seal a four-lumen fluted balloon to a shaft containing only a guidewire lumen. In yet another embodiment (not shown), where the catheter type is a "tip RX" (i.e., the guidewire lumen does not pass through any of the balloon lumens), the proximal seal geometry is used to seal a four-lumen fluted balloon to a shaft containing only a radiation source lumen.

Referring to FIG. 18, a cross sectional view of a multi-lumen fluted balloon for treating a body vessel 16 in the vascular system is shown. Balloon 10 includes a central lumen 12 and a plurality of outer lumens (or lobes) 11 disposed around the central lumen 12. The outer lumens 11 are integrally coupled with the central lumen 12 so as to form the multi-lumen balloon 10. Each of the balloon outer lumens 11 has an inner radial length (or diameter) 18 and an outer diameter 15, defining balloon outer lumen walls 17. The walls 17 of balloon outer lumens 11 are made very thin to allow proper inflation and deflation of outer lumens 11.

The multi-lumen balloon 10 is manufactured of balloon materials, such as Pebax™, nylon, polyethylene, polyurethane, or polyester. Materials for use in

009720" 1803530

fabricating the multi-lumen balloon 10 of the present invention are selected by considering the properties and characteristics (e.g., softness, durability, low stiffness) required by angioplasty balloons, as well as considering properties necessary for successful balloon fabrication (e.g., balloon material compatible with other catheter materials and bonding process, material extruding well, etc.).

In the embodiment illustrated in FIG. 17, a radiation source lumen 22 is placed into the central lumen 12 of the fluted multi-lumen balloon 10, the radiation source lumen 22 extending lengthwise through the central lumen 12. A guidewire lumen 21 is also placed into one of the balloon's outer lumens 11 (third outer lumen 11 of the balloon is hidden in FIG. 17), the guidewire lumen 21 extending lengthwise through the balloon outer lumen. The balloon outer lumen 11 containing the guidewire lumen 21 is labeled the guidewire outer lumen. Both the radiation source lumen 22 and the guidewire lumen 21 are manufactured as co-extrusions having an inner layer made of a material such as polyethylene and an outer layer made of a material such as Pebax, nylon, or Primacor.

A first mandrel 22a is then inserted through the radiation source lumen 22 and a second mandrel 21a is inserted through the guidewire lumen 21. It should be noted that if the catheter type does not require for a guidewire lumen 21 to extend through the multi-lumen balloon (for example, a "tip RX" catheter type or a catheter assembly having slideable distal and proximal seals, as discussed above), the second mandrel 21a may not be necessary and would not have to be inserted through one of the balloon outer lumens 11. For balloon catheter embodiments

where a radiation source lumen is not used (i.e., a radiation source would be positioned directly within the balloon central lumen during the intervascular radiotherapy procedure), the first mandrel 22a may be inserted directly through the balloon central lumen 12.

5 After the first mandrel 22a is inserted through the radiation source lumen 22 and the second mandrel 21a is inserted through the guidewire lumen 21, the two outer lumens 11 not occupied by the guidewire lumen 21 are compressed so as to give the outer lumens 11 (and thus the balloon proximal seal) a more compact configuration. Note that FIG. 18 shows a cross-section of the outer lumens 11
10 shape before the outer lumens are compressed. As part of the compressing operation, the proximal ends of the two outer lumens 11 are flattened (see FIG. 19a), thus forming flattened outer lumens.

 If a more packed configuration is desired for the flattened outer lumens 11, the ends 53 of the flattened outer lumens 11 are folded back over themselves (see
15 FIG. 19c), thus creating folded outer lumens. It is necessary to fold the ends 53 of the flattened outer lumens 11 back over themselves to ensure that there is enough balloon material outside of the inflation lumens 54b, 55b (shown in FIG. 20a, and discussed in more detail below) of the outer lumens 11 to maintain the inflation pressure. Alternative folding patterns of the flattened outer lumens may also be
20 used if there is ample thickness in the catheter outer member 46 to ensure that the inflation lumens (54b, 55b) will not leak. In one approach, the flattened outer lumens 11 may be left in the flattened profile shown in FIG. 19a or both ends 53 of

the outer lumens may be folded towards the guidewire outer lumen (i.e., the outer lumen 11 containing the guidewire lumen 21) (see FIG. 19b). Folding the flattened outer lumens 11 may be performed manually, using full automation techniques, or using a combination of manual and automated sub-steps.

5 If the flattened outer lumens are folded manually, many different approaches may be taken. For example, to achieve the embodiment shown in FIG. 19b, the flattened outer lumens are folded by simply using the thumb and forefinger to push down (or up, depending on the up or down orientation of the guidewire outer lumen) the two flattened outer lumens. The embodiment shown in FIG. 19c is done by
10 using a pair of tweezers to fold over the ends of each of the two flattened outer lumens (one side at the time) until the desired fold configuration is achieved.

 After folding the flattened balloon outer lumens 11, a catheter outer member 46 is placed over the central lumen 12 (with radiation source lumen 22) and the guidewire outer lumen 11 (with the guidewire lumen 21). The catheter outer
15 member 46 also overlaps the two outer lumens 11 of the multi-lumen balloon 10 not occupied by the guidewire lumen 21. The catheter outer member 46 may be manufactured from materials such as nylon, Pebax, polyurethane, etc.

 Inflation lumen mandrels 54a and 55a are then inserted to form and maintain individual lumens (54b, 55b) for inflation of the outer lumens 11. The inflation lumen
20 mandrels (54a, 55a) are generally inserted from the balloon distal end 28 (see FIG. 17), however, the insertion of the inflation lumen mandrels may also be accomplished from the balloon proximal end 29.

009720-1303360

The inflation lumen mandrels 54a (shown in FIG. 20d) have a “football”-
shape cross-section 54aa to better contour with the shape of the outer member 46
and prevent leaking of the inflation medium 18 through the inflation lumens 54a. In
current prior art balloon seal processes, which use mandrels having a straight
5 edged configuration (such as a flattened round wire mandrel), seal leaking can
occur because the “sharp” edges of the flattened round wire mandrels protrude out
of the seal, thus causing the inflation medium to leak out of the seal.

Referring to FIG. 20d, the inflation lumen mandrels 54a include a shaft 54a1
having a substantially football-shaped cross section. The shaft 54a1 has a solid
10 center, however, it may also have a hollow center 54a2 extending lengthwise
therein. The “football” shaped inflation lumen mandrels 54a are also symmetrical
(i.e., they do not have a “front”, “back”, “top”, or a “bottom”) to eliminate any
dependence on a specific orientation and for ease of use during the manufacture of
the proximal seal. The dimensions (i.e., length and cross-section “diameter”) of the
15 inflation lumen mandrels 54a vary depending for example, on the diameter of the
balloon lumens, the type of material the mandrel is made of, etc.

Referring to FIGS. 20a-20c, FIG. 20a shows a cross-section view of the
completed balloon proximal seal showing the inflation lumens 54b created by the
“football” shaped inflation lumen mandrels 54a for the two outer lumens not
20 occupied by the guidewire lumen, and the inflation lumen 55b created by the
flattened round wire inflation lumen mandrel 55a for the guidewire lumen 21. The
flattened round wire inflation lumen mandrel 55a can be replaced with a “football”

shaped inflation mandrel 56a (see FIG. 20b) or a triangular shaped mandrel 56b (see FIG. 20c). Following the insertion of the first and second mandrels (21a, 22a) to retain the radiation source lumen 22 and the guidewire lumen 21, and the inflation lumen mandrels (54a, 55a) to retain the inflation lumens (54b, 55b), the proximal end of the multi-lumen fluted balloon 10 is bonded to the distal end of the catheter outer lumen 46.

For the embodiment shown in FIG. 20a, a square-wave laser pattern bond is used to bond the outer member 46 to the balloon 10. A heat shrink tube 57b (shown in FIG. 21c) is temporarily used during the square-wave laser bond process.

The heat shrink tube 57b is positioned over the balloon catheter “proximal seal assembly”, which includes the proximal end of the multi-lumen balloon (with the radiation source lumen and the guidewire lumen if catheter assembly so requires it), the distal end of the catheter outer member, and all the mandrels. When heat from the laser beam is applied onto the heat shrink tube 57b, the tube compresses radially onto the balloon catheter proximal seal assembly. The shrink tube compression causes the materials of the balloon proximal end and the outer member distal end to closely fuse together, creating a leak-tight balloon proximal seal. The heat shrink tube is then removed. It should be noted that the heat shrink tubing may be substituted with heat shrink materials having other shapes, such as heat shrink sheaths, etc.

The shrink tubing is made from materials known in the art of catheter balloon manufacture. For one embodiment, the shrink tubing has a diameter 57b1 of 2.5

mm, however, the diameter 57b1 of the shrink tubing to be used depends on a number of factors, such as the size of the balloon catheter to be manufactured, the degree of folding performed on the balloon outer lumens, whether the balloon catheter includes a radiation source lumen and /or a guidewire lumen extending
5 through the balloon, etc.

In the present invention, laser bonding techniques, such as laser bonding using a square-wave laser pattern (or design) are desired. However, bonds may also be done using other balloon bonding techniques known in the art, such as thermal bonding, ultrasonic bonding, adhesive bonding (for example using a glue-
10 type material), or other conventional means.

Following the laser bonding of the outer member 46 to the balloon 10, the inflation lumen mandrels 54a and 55a are removed from the balloon proximal seal assembly.

Given the “egg-shape” like configuration, the completed balloon proximal
15 seal cross-section may have a “small diameter” 46d1 (i.e., measured horizontally across the seal) in a range of approximately 35-50 mm, while the “large diameter” 46d2 (i.e., measured vertically across the seal) in a range of approximately 60-80 mm. In one embodiment, the proximal seal cross section has a “small diameter” 46d1 of about 47 mm and a “large diameter” 46d2 of about 62 mm.

20

“Football”-shaped mandrels

As mentioned above, “football”-shaped mandrels are used in the manufacture of the multi-lumen balloon centering catheter proximal seal. Mandrels having a “football”-shape cross-section are not just limited to the manufacture of centering catheters. “Football”-shape cross section mandrels can also be used in
5 fabricating other medical interventional devices, such as atherectomy devices, delivery systems (stent or drug) and other devices requiring a tight seal configuration.

Referring to FIG. 20d, a “football”-shape cross section mandrel includes a shaft 54a1 having a substantially football-shaped cross section. The shaft 54a1 has
10 a solid center, however, it may also have a hollow center 54a2 extending lengthwise therein. The “football”-shaped mandrel shaft 54a1 is made to be symmetrical (i.e., the shaft does not have a “front”, “back”, “top”, or a “bottom”) to eliminate any dependence on a specific orientation and for ease of use. The “football”-shaped mandrel 54a may be manufactured out of metal, of a non-stick material such as
15 Teflon, or of any non-metal materials that will not melt at the same temperature as the materials used for manufacturing the particular medical device. The dimensions (i.e., length and cross-section “diameter”) of the “football”-shaped mandrel 54a vary depending for example, on the diameter of the balloon lumens, the type of material the mandrel is made of, etc. In one embodiment, the “football”-shaped mandrel 54a
20 has a “large diameter” 54aa1 (see FIG 20d) in a range of approximately 4/1000 – 30/1000 in. to a “small diameter” 54aa2 in a range of approximately 2/1000-20/1000 in.

Balloon Distal Seal

A unique balloon distal seal geometry used to seal a multi-lumen fluted balloon to a catheter shaft is described. The present invention provides a solution to the problem of bundling together a multi-lumen shaft at the distal end of a multi-lumen balloon without using additional materials that could increase the stiffness of the distal tip. The balloon distal seal is completed following the completion of the balloon proximal seal (as discussed above).

In one embodiment (described herein), the balloon distal seal geometry is used to seal a four-lumen fluted balloon to a shaft containing both a radiation source lumen and a guidewire lumen extending through the balloon lumens. It should be noted that for a "tip RX" catheter type (i.e., where the guidewire lumen does not extend through any of the balloon lumens), the balloon distal seal geometry is used to seal a four-lumen fluted balloon to a shaft containing a radiation source lumen and a short guidewire lumen distally positioned to the multi-lumen balloon. In another embodiment (not shown), where the radiation source is used without a radiation source lumen, the balloon distal seal geometry is used to seal a four-lumen fluted balloon to a shaft containing only a guidewire lumen.

Referring to FIG. 18, a cross sectional view of a multi-lumen fluted balloon for treating a body vessel 16 in the vascular system is shown. Balloon 10 includes a central lumen 12 and a plurality of outer lumens (or lobes) 11 disposed around the central lumen 12. The outer lumens 11 are integrally coupled with the central lumen

12 so as to form the multi-lumen balloon 10. The multi-lumen balloon 10 is manufactured of balloon materials, such as Pebax™, nylon, polyethylene, polyurethane, or polyester.

Referring to FIG. 17, a radiation source lumen 22 is placed into the central lumen 12 of the fluted multi-lumen balloon 10, the radiation source lumen 22 extending lengthwise through the central lumen 12. A guidewire lumen 21 is also placed into one of the balloon's outer lumens 11 (third outer lumen 11 of the balloon is hidden in FIG. 17), the guidewire lumen 21 extending lengthwise through the balloon outer lumen. The balloon outer lumen 11 containing the guidewire lumen 21 is labeled the guidewire outer lumen. Both the radiation source lumen 22 and the guidewire lumen 21 are manufactured as co-extrusions having an inner layer made of a material such as polyethylene and an outer layer made of a material such as Pebax, nylon, or Primacor.

Referring to FIG. 21a, a completed balloon distal seal 28 is illustrated. As discussed above, the balloon distal seal is completed following the completion of the balloon proximal seal.

To complete the distal seal 28 for a multi-lumen balloon radiation centering catheter, the following sub-steps are performed. First, a first source mandrel 22a is inserted into the radiation source lumen 22 and a first guidewire mandrel 21a is inserted into the guidewire lumen 21. Mandrels 22a and 21a form a first set of source and guidewire mandrels. In one embodiment of this invention, the first source mandrel 22a has a diameter of 0.0225 in., while the first guidewire mandrel

21a has a diameter of 0.017 in. The diameters of the first source and guidewire mandrels may vary depending on a number of factors, such as the type of source used, the size of the multi-lumen balloon when inflated (e.g., 2 mm, 3 mm balloon overall diameter), etc.

5 Next, a soft tip material 26 is placed over the first guidewire mandrel 21a so as to overlap the guidewire lumen 21. The soft tip material 26 is attached to the distal end 27 of the guidewire lumen 21 to improve trackability and reduce trauma to the body vessel. The length of the soft tip 26 depends on the type of catheter design used. However, when completed, the length of the soft tip 26 is generally in
10 a range of approximately 0.5 mm to 10 mm. The soft tip is manufactured from materials generally known in the field of balloon angioplasty.

 Next, to prepare the balloon distal seal for laser bonding, a first shrinkable material, such as a shrink tube 57b is positioned over the balloon distal seal sub-assembly. The sub-assembly includes the distal end of the multi-lumen balloon
15 (with the radiation source lumen and the guidewire lumen, if catheter assembly so requires it) and both mandrels (21a, 22a). The distal seal sub-assembly is then fastened using a hot box device (not shown). The balloon distal end 34b is then sealed using a laser device (not shown). It should be noted that the heat shrink tube 57b is only temporarily used during the laser bond process.

20 When heat from the laser beam is applied onto the heat shrink tube, the tube compresses radially onto the balloon catheter distal seal assembly. The shrink tube compression causes the materials of the balloon distal end 34b to closely fuse

together, creating a leak-tight balloon distal seal. The heat shrink tube 57b is then removed.

It should be noted that the heat shrink tube may be substituted with heat shrink materials having other shapes, such as heat shrink sheaths, etc. The shrink tube 57b is made from materials known in the art of catheter balloon manufacture. For one embodiment, the shrink tube 57b has a diameter 57b1 of 2.5 mm, however, the diameter of the shrink tube to be used depends on a number of factors, such as the size of the balloon catheter to be manufactured, the degree of folding performed on the balloon outer lumens, whether the balloon catheter includes a radiation source lumen and /or a guidewire lumen extending through the balloon, etc.

After removing the first shrink tube 57b, a tip jacket 57 is placed over both the guidewire lumen 21 and radiation source lumen 22. A second shrinkable material, such as a shrink tube 57c is placed over the tip jacket 57. The second shrink tube 57c is made from materials known in the art of catheter balloon manufacture. For one embodiment, the shrink tubing 57c has a diameter 57b1 of 2.0 mm, however, the diameter may be in a range of approximately 1.0-3.0 mm. The distal seal sub-assembly (with the tip jacket 57) is then sealed using a laser device (not shown).

The multi-lumen fluted balloon distal seal sub-assembly is laser sealed using a conventional helical-wave laser design. In the present invention, laser sealing or bonding techniques such as the square-wave laser design may be desirable. However, bonds may also be done using other balloon bonding techniques known

in the art, such as thermal or ultrasonic welds, adhesive bonds (for example glue), or other conventional means.

Following the laser bonding of the tip jacket 57, the second shrink tubing 57c is removed. The first set of source and guidewire mandrels (22a, 21a) is then replaced with a second set of source and guidewire mandrels (22aa, 21aa) having smaller diameters than mandrels 22a and 21a. In one embodiment of this invention, the second source mandrel 22aa has a diameter of 0.0205 in., while the second guidewire mandrel 21aa has a diameter of 0.016 in. The diameters of the second source and guidewire mandrels may vary depending on a number of factors, such as the type of source used, the size of the multi-lumen balloon when inflated (e.g., 2 mm, 3 mm balloon overall diameter), etc.

Once the source and guidewire mandrels are replaced with smaller-diameter mandrels, a tip-forming sheath 57a (shown in FIG. 21b) is placed over the laser-sealed tip jacket 57. Using the tip-forming sheath 57a, a guidewire soft tip (shown in FIGS. 1, 6, 10, and 13) is formed using by placing the balloon seal sub-assembly into a hot box (not shown). At the completion of the distal seal 28, the second source mandrel 22aa and the second guidewire mandrel 21aa are removed from the balloon seal sub-assembly.

Alternative Source Mandrel Designs for Distal Seal

The source mandrels presented above refer to a mandrel design having a circular cross-section. However, the circular cross-section design for the source

mandrels may be substituted by using two additional source mandrel designs: (1) a tapered-shape mandrel, and (2) a ramped-shape mandrel. These two embodiments of this invention are now discussed

Tapered Mandrel

5 Referring to FIG. 21d, a tapered mandrel is formed by having a gradual taper of one end of the mandrel (22a or 22aa) while keeping the round cross-sectional shape concentric to the mandrel. The tapered mandrel has a gradual taper length 21a1 that may vary from 0 cm (i.e., flat ended mandrel) to a taper length 21a1 of 10 cm. This gradual taper shapes the end of the source lumen 22 to direct the
10 radiation source (such as a wire) directly at center of the lumen.

Ramped Mandrel

Referring to FIG. 21e, a ramped mandrel (22a or 22aa) is shown. In the ramped mandrel design, a round is first made to one end of the mandrel. Then a flat ramp is cut into the same end of the mandrel on one side (see FIG. 21e). The
15 ramped mandrel has a ramp length 22a2 that may vary from 0 cm (i.e., flat ended mandrel) to a ramp length 22a2 of 5 cm. This ramped feature shapes the end of the source lumen to direct the source wire slightly downwards and away from exiting through the top of the lumen.

20

Method of manufacture

Multi-Lumen Tubing

Referring to FIGS. 22a-25a, the multi-lumen fluted balloon 10 of this invention is fabricated by blowing a multi-lumen tubing 60 created using an extrusion process. The multi-lumen extruded tubing 60 has a tubing body 61, a central lumen 62, and at least one outer lumen 63 disposed adjacent to the central lumen 62. Generally, a plurality of outer lumens 63 are disposed adjacent to the central lumen 62. The outer lumen 63 is coupled with the central lumen 62 by a shared wall 67 (as shown in FIGS. 22a-25a). In one embodiment, the multi-lumen tubing 60 has three outer lumens 63 disposed adjacent to the central lumen 62.

Referring the FIGS. 23a and 24a, in one embodiment of the present invention, the multi-lumen tubing 60 has at least one outer lumen 63 disposed adjacent to the central lumen 62. The outer lumen 63 is coupled with the central lumen 62 by a shared wall 67. The multi-lumen tubing 60 further includes an undercut radius region 65 disposed between the central lumen 62 and the outer lumen 63. The shared wall 67 may have a shared wall thickness 67b in a range of approximately 50%-200% of the outer lumen wall thickness 67c (as shown in FIG. 23a). In one embodiment, the shared wall 67 may have a shared wall thickness 67b in a range of approximately 80%-120% of the outer lumen wall thickness 67c (as shown in FIG. 24a).

Referring to FIG. 22a, in another embodiment of the present invention, the multi-lumen tubing 60 has at least one outer lumen 63 disposed adjacent to the central lumen 62. The outer lumen 63 is coupled with the central lumen 62 by a

shared wall 67. The multi-lumen tubing 60 includes a fillet radius region 66 instead of the undercut region 65 shown in the embodiments of FIG. 23a and 24a. The fillet radius region 66 is disposed between the central lumen 62 and the outer lumens 63. The shared wall 67 may have a shared wall thickness 67b in a range of approximately 50%-200% of the outer lumen wall thickness 67c. In one embodiment, the shared wall 67 may have a shared wall thickness in a range of approximately 80%-120% of the outer lumen wall thickness 67c (as shown in FIG. 23a).

Referring to FIG. 25a, in a third embodiment of the present invention, the multi-lumen tubing 60 includes a standoff region 64 disposed between the central lumen 62 and the outer lumens 63. In this configuration, the standoff region 64 is the same as the shared wall 67 (i.e., the standoff region 64 has the same shape and length as the shared wall 67). The standoff region 64 may have a standoff region thickness 67bb in a range of approximately 50%-200% of the outer lumen wall thickness 67c. In one embodiment, the standoff region 64 may have a standoff region thickness 67bb in a range of approximately 80%-120% of the outer lumen wall thickness 67c (as shown in FIG. 25a).

The multi-lumen tubing 60 of the present invention may have an overall diameter 68 in a range of approximately about 20/1000 in. to 50/1000 in. In one embodiment of this invention, the multi-lumen tubing 60 may have an overall diameter 68 in a range of approximately about 34/1000 in. to 48/1000 in.

The central lumen 62 of the multi-lumen tubing 60 may have an inner diameter (69a-69d, as shown in FIGS. 22a-25d) in a range of approximately about 7/1000 in. to 13/1000 in. In one embodiment of this invention, the central lumen 62 of the multi-lumen tubing 60 has an inner diameter of about 10/1000 in.

5 The outer lumens 63 of the multi-lumen tubing 60 may have an outer lumen wall thickness 67c in a range of approximately 2/1000 in. to 8/1000 in. In one embodiment of this invention, the outer lumens 63 may have an outer lumen wall thickness 67c in a range of approximately 3.5/1000 in. to 6/1000 in.

10 The multi-lumen tubing 60 is manufactured using balloon materials, such as resin, Pebax™, nylon, polyethylene, polyurethane, or polyester. Materials for use in fabricating the multi-lumen extrusion tubing 60 of the present invention are selected by considering the properties and characteristics (e.g., softness, durability, low stiffness) required by angioplasty balloons, as well as considering properties necessary for successful balloon fabrication (e.g., balloon material compatible with
15 other catheter materials and bonding process, material extruding well, etc.).

Multi-Lumen Tubing - Method of manufacture: Extrusion

FIG. 26 is a flow chart illustrating the steps of fabricating a multi-lumen extruded tubing of one embodiment of the present invention, such as the multi-lumen extruded tubing for the radiation centering catheter shown in FIGS. 1, 6, 10,
20 and 13.

Referring to FIG. 26, the first step in the extruded tubing manufacture process is to select an appropriate material from which the extruded tubing (and

thus the balloon) will be manufactured (step 100). Recall that the multi-lumen extruded tubing is made of balloon materials known in the art of balloon angioplasty, such as Pebax™, nylon, polyethylene, polyurethane or polyester. Generally, any resin-type material may be used to manufacture the multi-lumen extruded tubing.

- 5 Materials for use in fabricating the multi-lumen extruded tubing of the present invention are selected by considering the properties and characteristics (e.g., softness, durability) required by angioplasty balloons, as well as considering properties necessary for successful balloon fabrication (e.g., balloon material compatible with other catheter materials and bonding process, material extruding
- 10 well, etc.).

At step 200 in the multi-lumen extruded tubing fabrication process, the resin material is placed into a hopper (or a similar purpose receptacle) and is then gradually brought to a molten state.

- The next three steps (Steps 300, 400, and 500) are performed concurrently
- 15 during the multi-lumen extruded tubing manufacture process. In Step 300, the molten resin material is run through a tip and die assembly such that at least one multi-lumen shaft is formed. As part of Step 400, a pressurized medium (such as air or other gas) is applied into each of the lumens of the multi-lumen shaft (or the plurality of single lumen shafts) formed as part of Step 300 to maintain and/or
- 20 control the inner diameter of the lumens (or bores) 63 formed lengthwise along the centerline of the shaft (or along a centerline of each of the plurality of shafts). If a pressurized gas is used, the pressurized gas applied to the plurality of resin material

shafts may done at a pressure in a range of approximately 0-30 inches of water. In one embodiment, the pressurized gas applied to the plurality of resin material shafts is at a pressure of 2 inches of water.

Step 500 includes pulling the shaft (or depending on the extrusion die configuration, a plurality of shafts) away from the extrusion die (using a puller or similar device) so as to form the multi-lumen extruded tubing having the desired lumen inner diameter, lumen wall thickness, shared wall thickness, outer tubing shape, etc. Pulling the plurality of shafts away from the extrusion die (Step 500) may be done while the resin material is at a melt temperature in the range of about 370 °F to 440 °F. In one embodiment, pulling the plurality of shafts away from the extrusion die is done while the resin material is at a melt temperature in the range of about 380 °F to 410 °F. Pulling the plurality of resin material shafts away from the extrusion die may be done at a pulling rate of about 25-100 feet per minute. In one embodiment, pulling the plurality of resin material shafts away from the extrusion die is done at a pulling rate of about 45-65 feet per minute.

For extrusion die configurations that permit a plurality of shafts to be formed instead of a single shaft (as discussed below), Step 500 includes pulling the plurality of shafts away from the extrusion die so as to cause the plurality of shafts to fuse together lengthwise into the multi-lumen extrusion tubing having a central lumen and at least one outer lumen disposed adjacent to the central lumen.

Referring to FIGS. 22b-25b, several embodiments of a tip and die assembly of the present invention are shown. Each tip and die assembly includes an

extrusion die (shown as 70, 170, 270, 370 in FIGS. 22b-25b) and a plurality of extrusion tip hypo-tubes (identified as 71a, 171a, 271a, 371a in the figures) through which a pressurized medium (such as air, an inert gas, liquid, etc.) is introduced into the shaft's lumen to maintain and/or control the inner diameter of the lumen. The

5 extrusion die may have a single common exit hole (item 76 in FIG. 22b and item 376 in FIG. 25b) or a plurality of exit holes (items 171, 172 in FIG. 23b and items 71, 72 in FIG. 24b). The hypo-tubes may take the form of mandrels (items 271a, 171a, 71a, and 371a in FIGS. 22b-25b) having a bore extending lengthwise through the center of the mandrels.

10 Continuing with reference to FIG. 22b, the extrusion die 270 is used in the manufacture of the multi-lumen extruded tubing 60 shown in FIG. 22a. The extrusion die 270 includes a single common exit hole 76 having a profile such that a multi-lumen extruded tubing 60 with a fillet radius region 66 disposed between the central lumen 62 and the plurality of outer lumens 63 is formed. The extrusion die

15 270 may be manufactured out of a metal, a hard plastic, or any other type of material used in medical extrusion tubing processes. Using a die with a single common exit hole simplifies the overall tubing extrusion process, thus permitting a multi-lumen single shaft to be more easily manufactured.

Referring to FIG. 23b, in a second embodiment of this invention, the

20 extrusion die 170 is used in the manufacture of the multi-lumen extruded tubing 60 shown in FIG. 23a. The extrusion die 170 has at least one outer exit hole 171 disposed around a central exit hole 172. The outer exit hole 171 may be positioned

at various distances 175 from the central exit hole 172. It may be desirable to place the outer exit hole 171 as close as possible to the central exit hole 172 in order to minimize the amount of resin material of the shared wall thickness 67b (shown in FIG. 23a). Having less resin material as part of the shared wall permits the multi-lumen tubing to blow better during the balloon forming process and ultimately leads to a less stiff balloon. The extrusion die 170 may be manufactured out of a metal, a hard plastic, or any other type of material used in medical extrusion tubing processes.

Referring to FIG. 24b, in a third embodiment of this invention, the extrusion die 70 is used in the manufacture of the multi-lumen extruded tubing 60 shown in FIG. 24a. The extrusion die 70 includes at least one outer exit hole 71 disposed around to a central exit hole 72. The outer exit hole 71 has a substantially flat shape across a part 73 of a periphery where the outer exit hole 71 is disposed adjacent to the central exit hole 72. The central exit hole 72 also has a substantially flat shape across a part 74 of a periphery where the central exit hole 72 is disposed adjacent to the outer exit hole 71.

The extrusion die 70 may be configured so that the outer exit hole 71 could be positioned at various die region thicknesses (or distances) 75 on the die region between the central exit hole 72 and outer exit hole 71. The die region thickness 75 may range from 0 in. to 10/1000 in. In one embodiment, the die region thickness 75 between the central exit hole 72 and the outer exit hole 71 is about 5/1000 in. It may be desirable to keep the die region thickness 75 to a thickness width such that

when formed, the shared wall thickness 67b of the multi-lumen 60 is approximately equal to the outer lumen wall thickness 67c (see FIG. 24a). Having a shared wall thickness 67b in a range of approximately about 80% to 120% of the outer lumen wall thickness 67c minimizes the resin material of the shared wall and permits the multi-lumen tubing to blow better during the balloon forming process and ultimately leads to a less stiff balloon. The extrusion die 70 may be manufactured out of a metal, a hard plastic, or any other type of material used in medical extrusion tubing processes.

Referring to FIG. 25b, in a fourth embodiment of this invention, the extrusion die 370 is used in the manufacture of the multi-lumen extruded tubing 60 shown in FIG. 25a. The extrusion die 370 includes a single common exit hole 376 having a profile such that a multi-lumen extruded tubing 60 with at least one standoff region 64 disposed between the central lumen 62 and the outer lumens 63 is formed (see FIG. 25a). The extrusion die 370 may be manufactured out of a metal, a hard plastic, or any other type of material used in medical extrusion tubing processes. Using a die with a single common exit hole and having a profile with at least one standoff region minimize the amount of resin material between the central lumen 62 and plurality of outer lumens 63 (shown in FIG. 25a). Having less resin material permits the multi-lumen tubing 60 to blow better during the balloon forming process and ultimately leads to a less stiff balloon. Furthermore, using a die with a single common exit hole simplifies the overall tubing extrusion process, thus permitting a multi-lumen single shaft to be more easily manufactured.

The next step in the fabrication process, Steps 610 and 620, is to form the final balloon shape with multiple lumens. This is achieved by placing the multi-lumen extruded tubing obtained after completion of Steps 300-500 into a steel cylinder that is configured to have the appropriate shape of the final balloon.

5 Once the multi-lumen balloon is formed and shaped to the desired dimensions and configurations, the next steps include preparing the balloon and catheter assembly for the balloon proximal seal (Step 710) and performing the balloon proximal seal (Step 720). Step 810 includes preparing the balloon and catheter assembly for the balloon distal seal, while Step 820 includes performing
10 the balloon distal seal.

In one embodiment of the present invention, laser bonding techniques are used to perform the proximal and distal seals. However, any seal bonding techniques known in the art of manufacture of angioplasty balloon catheters may be employed to achieve the seals.

15

Multi-Lumen Tubing – Alternate Method of manufacture: Dip Coating

An alternate method of manufacture of the multi-lumen balloon is by using a “Dip Coating” process. A description of this process and how the multi-lobed, multi-lumen balloon is made is presented herein.

20 First, a “mandrel” is obtained. The mandrel includes component elements (such as pins) that are sized and arranged such that they define the lumens (i.e., interior void spaces) of the intended multi-lumen balloon.

Next, the physical balloon elements (i.e., balloon lumens, thickness of balloon walls, etc.) are defined by applying a thin film of a pre-selected polymer (analogous to applying paint) on and about the pin. In one embodiment, the application of the thin film polymer is achieved by immersing the mandrel into a bath of the desired polymer. The polymer may be any polymer with properties that would lend themselves to dip coating such as the ability to go into solution or suspension with subsequent recovery of adequate film properties. Materials already used in this manner are for example: poly-urethanes, siloxanes or silicones, and latexes.

The thickness of the film (balloon wall) may be controlled by such factors as the viscosity of the bath solution and/or the number of times the mandrel is dipped into the solution. The "carrier" or "solvent" is then driven off (evaporated) by normal means such as time in ambient air or forced convection with or without added heat.

The balloon, if appropriate to the polymer selected, may be further processed to impart enhanced or additional properties such as irradiation to increase cross-linking. This can be achieved either before or after removing from the mandrel as appropriate to the material and/or properties and/or process.

In the next step, the film that is the balloon is then "stripped off" the mandrel through any appropriate means such as: using compressed air ported through the pins that make up the mandrel, swelling the balloon material with some other solvent which frees the balloon material from the mandrel and this solvent is then driven off returning the balloon to the original dimensions, mechanically stripping off the balloon, etc.

Finally, the balloon is trimmed and prepped as necessary for integration with the remaining catheter components.

A multi-lumen balloon for use in a fluted balloon centering catheter and method for providing the same has been described. Although specific
5 embodiments, including specific parameters, methods, and materials have been described, various modifications to the disclosed embodiments will be apparent to one of ordinary skill in the art upon reading this disclosure. Therefore, it is to be understood that such embodiments are merely illustrative of and not restrictive on the broad invention and that this invention is not limited to the specific embodiments
10 shown and described.

0097607305960

1. A multi-lumen balloon radiation centering catheter assembly, comprising:

- a multi-lumen balloon having a plurality of inflatable outer lumens disposed around a central lumen, the plurality of outer lumens integrally coupled with the central lumen so as to form the multi-lumen balloon; and

5 - a catheter shaft disposed proximate to the balloon, the catheter shaft including an inner lumen longitudinally extending through at least a portion of the catheter shaft proximate the balloon and connected to the central lumen, the inner lumen adapted for receiving a radiation source lumen, the inner lumen further adapted for receiving a guidewire lumen for positioning the multi-lumen balloon radiation

10 centering catheter within a body vessel, wherein the guidewire lumen extends lengthwise through one of the plurality of outer lumens.

1 2. The multi-lumen balloon radiation centering catheter assembly of claim 1,
2 wherein the inner lumen is further adapted for receiving a plurality of inflation
3 lumens that are in fluid communication with the plurality of outer lumens to allow an
4 inflation medium to enter and inflate the plurality of outer lumens so as to cause the
5 radiation source lumen to be centered within a body vessel.

1 3. The multi-lumen balloon radiation centering catheter assembly of claim 2,
2 wherein each outer lumen is inflatable to different inflation pressures.

1 4. The multi-lumen balloon radiation centering catheter assembly of claim 1,
2 wherein the inner lumen serves as an inflation lumen for the plurality of outer
3 lumens.

1 5. The multi-lumen balloon radiation centering catheter assembly of claim 1,
2 further comprising a catheter outer member coupled with the catheter shaft.

1 6. The multi-lumen balloon radiation centering catheter assembly of claim 5,
2 wherein the catheter outer member includes an outer member lumen extending
3 through at least a portion of the catheter outer member and connected to the
4 catheter shaft inner lumen, the outer member lumen adapted for receiving a inflation
5 lumen that is in fluid communication with the plurality of outer lumens for inflating
6 the multi-lumen balloon.

1 7. The multi-lumen balloon radiation centering catheter assembly of claim 1,
2 wherein the radiation source lumen extends lengthwise through the central lumen of
3 the multi-lumen balloon.

1 8. The multi-lumen balloon radiation centering catheter assembly of claim 7,
2 wherein the plurality of outer lumens have a plurality of proximal ends and distal
3 ends coupled with the radiation source lumen so as to form a balloon proximal seal
4 and a balloon distal seal.

1 9. The multi-lumen balloon radiation centering catheter assembly of claim 8,
2 wherein a balloon treatment area is formed between the balloon proximal seal and
3 the balloon distal seal.

1 10. The multi-lumen balloon radiation centering catheter assembly of claim 9,
2 wherein the balloon treatment area has a fluted shape.

1 11. The multi-lumen balloon radiation centering catheter assembly of claim 1,
2 wherein the guidewire lumen extending lengthwise through one of the outer lumens
3 of the multi-lumen balloon is a standard rapid exchange guidewire lumen.

1 12. The multi-lumen balloon radiation centering catheter of claim assembly 1,
2 further comprising a soft tip coupled to a distal end of the guidewire lumen.

1 13 The multi-lumen balloon radiation centering catheter of claim assembly 8,
2 further comprising a distal marker and a proximal marker coupled with the radiation
3 source lumen and disposed within the balloon distal seal and the balloon proximal
4 seal.

1 14. The multi-lumen balloon radiation centering catheter assembly of claim 13,
2 wherein the distal marker is part of a radiation source lumen plug.

1 15. The multi-lumen balloon radiation centering catheter assembly of claim 1,
2 further comprising a radiation source disposed within the radiation source lumen.

1 16. The multi-lumen balloon radiation centering catheter assembly of claim 15,
2 wherein the radiation source comprises a gamma radiation-emitting radiation
3 source.

1 17. The multi-lumen balloon radiation centering catheter assembly of claim 15,
2 wherein the radiation source comprises a beta radiation-emitting radiation source.

1 18. The multi-lumen balloon radiation centering catheter assembly of claim 17,
2 wherein the radiation source comprises phosphorous-32.

1 19. The multi-lumen balloon radiation centering catheter assembly of claim 2,
2 wherein when inflated and engaged with the body vessel, the plurality of outer
3 lumens form straight longitudinal paths that allow for perfusion of blood past the
4 multi-lumen balloon.

1 20. The multi-lumen balloon radiation centering catheter assembly of claim 1,
2 wherein the plurality of outer lumens have equal diameters when inflated by an
3 inflation medium.

1 21. The multi-lumen balloon radiation centering catheter assembly of claim 1,
2 wherein the plurality of outer lumens have unequal diameters when inflated by the
3 inflation medium.

1 22. The multi-lumen balloon radiation centering catheter assembly of claim 9,
2 wherein the balloon treatment area has a longitudinal length in a range of
3 approximately 10-250 mm.

1 23. The multi-lumen balloon radiation centering catheter assembly of claim 9,
2 wherein the balloon treatment area has a longitudinal length in a range of
3 approximately 18-54 mm.

1 24. The multi-lumen balloon radiation centering catheter assembly of claim 9,
2 wherein the balloon treatment area has a combined diameter in a range of
3 approximately 1.5-10 mm when inflated by the inflation medium.

1 25. The multi-lumen balloon radiation centering catheter assembly of claim 9,
2 wherein the balloon treatment area has a combined diameter in a range of
3 approximately 1.5-4 mm when inflated by the inflation medium.

- 1 26. The multi-lumen balloon radiation centering catheter assembly of claim 1,
- 2 wherein the multi-lumen balloon is manufactured from a material selected from the
- 3 group consisting of resin, nylon and pebax.

1 27. A multi-lumen balloon radiation centering catheter assembly, comprising:
2 - a multi-lumen balloon having a plurality of inflatable outer lumens disposed
3 around a central lumen, the plurality of outer lumens integrally coupled with the
4 central lumen so as to form the multi-lumen balloon; and
5 - a catheter shaft disposed proximate to the balloon, the catheter shaft including
6 an inner lumen longitudinally extending through at least a portion of the catheter
7 shaft proximate the balloon and connected to the central lumen, the inner lumen
8 adapted for receiving a radiation source lumen, the inner lumen further adapted
9 for receiving a guidewire lumen for positioning the multi-lumen balloon radiation
10 centering catheter within a body vessel, wherein the guidewire lumen is
11 positioned distal to the multi-lumen balloon.

1 28. The multi-lumen balloon radiation centering catheter assembly of claim 27,
2 wherein the inner lumen is further adapted for receiving a plurality of inflation
3 lumens that are in fluid communication with the plurality of outer lumens to allow an
4 inflation medium to enter and inflate the plurality of outer lumens so as to cause the
5 radiation source lumen to be centered within a body vessel.

1 29. The multi-lumen balloon radiation centering catheter assembly of claim 28,
2 wherein each outer lumen is inflatable to different inflation pressures.

1 30. The multi-lumen balloon radiation centering catheter assembly of claim 27,
2 wherein the inner lumen serves as an inflation lumen for the plurality of outer
3 lumens.

1 31. The multi-lumen balloon radiation centering catheter assembly of claim 27,
2 further comprising a catheter outer member coupled with the catheter shaft.

1 32. The multi-lumen balloon radiation centering catheter assembly of claim 31,
2 wherein the catheter outer member includes an outer member lumen extending
3 through at least a portion of the catheter outer member and connected to the
4 catheter shaft inner lumen, the outer member lumen adapted for receiving a inflation
5 lumen that is in fluid communication with the plurality of outer lumens for inflating
6 the multi-lumen balloon.

1 33. The multi-lumen balloon radiation centering catheter assembly of claim 27,
2 wherein the radiation source lumen extends lengthwise through the central lumen of
3 the multi-lumen balloon.

1 34. The multi-lumen balloon radiation centering catheter assembly of claim 33,
2 wherein the plurality of outer lumens have a plurality of proximal ends and distal
3 ends coupled with the radiation source lumen so as to form a balloon proximal seal
4 and a balloon distal seal.

1 35. The multi-lumen balloon radiation centering catheter assembly of claim 34,
2 wherein a balloon treatment area is formed between the balloon proximal seal and
3 the balloon distal seal.

1 36. The multi-lumen balloon radiation centering catheter assembly of claim 35,
2 wherein the balloon treatment area has a fluted shape.

1 37. The multi-lumen balloon radiation centering catheter assembly of claim 27,
2 wherein the guidewire lumen is a tip rapid exchange guidewire lumen.

1 38. The multi-lumen balloon radiation centering catheter of claim assembly 27,
2 further comprising a soft tip coupled to a distal end of the guidewire lumen.

1 39 The multi-lumen balloon radiation centering catheter of claim assembly 34,
2 further comprising a distal marker and a proximal marker coupled with the radiation
3 source lumen and disposed within the balloon distal seal and the balloon proximal
4 seal.

1 40. The multi-lumen balloon radiation centering catheter assembly of claim 39,
2 wherein the distal marker is part of a radiation source lumen plug.

1 41. The multi-lumen balloon radiation centering catheter assembly of claim 27,
2 further comprising a radiation source disposed within the radiation source lumen.

1 42. The multi-lumen balloon radiation centering catheter assembly of claim 41,
2 wherein the radiation source comprises a gamma radiation-emitting radiation
3 source.

1 43. The multi-lumen balloon radiation centering catheter assembly of claim 41,
2 wherein the radiation source comprises a beta radiation-emitting radiation source.

1 44. The multi-lumen balloon radiation centering catheter assembly of claim 43,
2 wherein the radiation source comprises phosphorous-32.

1 45. The multi-lumen balloon radiation centering catheter assembly of claim 28,
2 wherein when inflated and engaged with the body vessel, the plurality of outer
3 lumens form straight longitudinal paths that allow for perfusion of blood past the
4 multi-lumen balloon.

1 46. The multi-lumen balloon radiation centering catheter assembly of claim 27,
2 wherein the plurality of outer lumens have equal diameters when inflated by an
3 inflation medium.

1 47. The multi-lumen balloon radiation centering catheter assembly of claim 27,
2 wherein the plurality of outer lumens have unequal diameters when inflated by an
3 inflation medium.

1 48. The multi-lumen balloon radiation centering catheter assembly of claim 35,
2 wherein the balloon treatment area has a longitudinal length in a range of
3 approximately 10-250 mm.

1 49. The multi-lumen balloon radiation centering catheter assembly of claim 35,
2 wherein the balloon treatment area has a longitudinal length in a range of
3 approximately 18-54 mm.

1 50. The multi-lumen balloon radiation centering catheter assembly of claim 35,
2 wherein the balloon treatment area has a combined diameter in a range of
3 approximately 1.5-10 mm when inflated by the inflation medium.

1 51. The multi-lumen balloon radiation centering catheter assembly of claim 35,
2 wherein the balloon treatment area has a combined diameter in a range of
3 approximately 1.5-4 mm when inflated by the inflation medium.

1 52. The multi-lumen balloon radiation centering catheter assembly of claim 27,
2 wherein the multi-lumen balloon is manufactured from a material selected from the
3 group consisting of resin, nylon and Pebax.

1 53. The multi-lumen balloon radiation centering catheter assembly of claim 3,
2 wherein the outer lumens are inflated at different inflation pressures to cause the
3 central lumen not to be centered within the body vessel.

1 54. A multi-lumen balloon radiation centering catheter assembly, comprising:

- 2 - a multi-lumen balloon having a plurality of inflatable outer lumens disposed
3 around a central lumen, the plurality of outer lumens integrally coupled with the
4 central lumen so as to form the multi-lumen balloon having a proximal seal end
5 and a distal seal end, the balloon further comprising a plurality of bores
6 communicating between the central lumen and the plurality of outer lumens; and
7 - a catheter shaft having a proximal end and a distal end, the catheter shaft
8 distal end coupled with the balloon proximal seal end, the catheter shaft
9 comprising an inner tubular member which extends coaxially within an outer
10 tubular member, the inner tubular member adapted for receiving a radiation
11 source lumen, the inner tubular member further adapted for receiving at least
12 one inflation lumen that is in fluid communication with the plurality of outer
13 lumens to allow an inflation medium to inflate the plurality of outer lumens so as
14 to cause the radiation source lumen to be centered within a body vessel.

1 55. The multi-lumen balloon radiation centering catheter assembly of claim 54,
2 wherein the inner tubular member is further adapted to receive a guidewire lumen
3 for positioning the multi-lumen balloon radiation centering catheter assembly within
4 the body vessel.

1 56. The multi-lumen balloon radiation centering catheter assembly of claim 55,
2 wherein the guidewire lumen extends lengthwise through the central lumen.

1 57. The multi-lumen balloon radiation centering catheter assembly of claim 54,
2 wherein the inner tubular member extends lengthwise through the central lumen.

1 58. The multi-lumen balloon radiation centering catheter assembly of claim 57,
2 wherein the plurality of outer lumens have a plurality of proximal and distal ends
3 coupled with the inner tubular member so as to form a fluted shape multi-lumen
4 balloon between the balloon distal seal end and balloon proximal seal end.

1 59. The multi-lumen balloon radiation centering catheter assembly of claim 57,
2 wherein the inner tubular member extending lengthwise through the central lumen
3 of the multi-lumen balloon is adapted to be attached with a tip rapid exchange
4 guidewire lumen for positioning the catheter within the body vessel.

1 60. The multi-lumen balloon radiation centering catheter assembly of claim 55,
2 further comprising a soft tip coupled to a distal end of the guidewire lumen.

1 61. The multi-lumen balloon radiation centering catheter assembly of claim 59,
2 further comprising a soft tip coupled to a distal end of the tip rapid exchange
3 guidewire lumen.

1 62. The multi-lumen balloon radiation centering catheter assembly of claim 54,
2 further comprising a distal marker and a proximal marker coupled with the radiation
3 source lumen and disposed within the distal seal end and the proximal seal end of
4 the multi-lumen balloon.

1 63. The multi-lumen balloon radiation centering catheter assembly of claim 62,
2 wherein the distal marker is part of a radiation source lumen plug.

1 64. The multi-lumen balloon radiation centering catheter assembly of claim 54,
2 further comprising a radiation source disposed within the radiation source lumen.

1 65. The multi-lumen balloon radiation centering catheter assembly of claim 64,
2 wherein the radiation source comprises a gamma radiation-emitting radiation
3 source.

1 66. The multi-lumen balloon radiation centering catheter assembly of claim 64,
2 wherein the radiation source comprises a beta radiation-emitting radiation source.

1 67. The multi-lumen balloon radiation centering catheter assembly of claim 66,
2 wherein the radiation source comprises phosphorous-32.

1 68. The multi-lumen balloon radiation centering catheter assembly of claim 54,
2 wherein when inflated and engaged with the body vessel, the plurality of outer
3 lumens form straight longitudinal paths that allow for perfusion of blood past the
4 multi-lumen balloon.

1 69. The multi-lumen balloon radiation centering catheter assembly of claim 54,
2 wherein a balloon treatment area is formed between the balloon distal seal end and
3 the balloon proximal seal end.

1 70. The multi-lumen balloon radiation centering catheter assembly of claim 54,
2 wherein the plurality of outer lumens have equal diameters when inflated by the
3 inflation medium.

1 71. The multi-lumen balloon radiation centering catheter assembly of claim 54,
2 wherein the plurality of outer lumens have unequal diameters when inflated by the
3 inflation medium.

1 72. The multi-lumen balloon radiation centering catheter assembly of claim 54,
2 wherein the catheter shaft is a standard rapid exchange type.

1 73. The multi-lumen balloon radiation centering catheter assembly of claim 54,
2 wherein the catheter shaft is a tip rapid exchange type.

1 74. The multi-lumen balloon radiation centering catheter assembly of claim 54,
2 wherein the catheter shaft is an over-the-wire catheter type.

1 75. The multi-lumen balloon radiation centering catheter assembly of claim 69,
2 wherein the balloon treatment area has a longitudinal length in a range of
3 approximately 10-250 mm.

1 76. The multi-lumen balloon radiation centering catheter assembly of claim 69,
2 wherein the balloon treatment area has a longitudinal length in a range of
3 approximately 18-54 mm.

1 77. The multi-lumen balloon radiation centering catheter assembly of claim 69,
2 wherein the balloon treatment area has a combined diameter in a range of
3 approximately 1.5-10 mm when inflated by the inflation medium.

1 78. The multi-lumen balloon radiation centering catheter assembly of claim 69,
2 wherein the balloon treatment area has a combined diameter in a range of
3 approximately 1.5-4 mm when inflated by the inflation medium.

1 79. The multi-lumen balloon radiation centering catheter assembly of claim 54,
2 wherein the multi-lumen balloon is manufactured from a material selected from the
3 group consisting of resin, nylon and pebax.

1 80. A multi-lumen balloon radiation centering catheter assembly, comprising:
2 - a multi-lumen balloon having a plurality of inflatable outer lumens disposed
3 around a central lumen, the plurality of outer lumens integrally coupled with the
4 central lumen so as to form the multi-lumen balloon having a proximal seal end
5 and a distal seal end; and
6 - a catheter shaft having a proximal end and a distal end, the catheter distal
7 end coupled with the balloon proximal seal end, the catheter shaft comprising an
8 inner tubular member which extends coaxially within an outer tubular member,
9 the inner tubular member adapted for receiving a radiation source lumen, the
10 inner tubular member further adapted for receiving at least one inflation lumen
11 that is in fluid communication with the plurality of outer lumens to allow an
12 inflation medium to inflate the plurality of outer lumens so as to cause the
13 radiation source lumen to be centered within a body vessel.

1 81. The multi-lumen balloon radiation centering catheter assembly of claim 80,
2 wherein the inner tubular member is further adapted to receive a guidewire lumen
3 for positioning the multi-lumen balloon radiation centering catheter assembly within
4 the body vessel.

1 82. The multi-lumen balloon radiation centering catheter assembly of claim 81,
2 wherein the guidewire lumen extends lengthwise through the central lumen.

1 83. The multi-lumen balloon radiation centering catheter assembly of claim 80,
2 wherein the inner tubular member extends lengthwise through the central lumen.

1 84. The multi-lumen balloon radiation centering catheter assembly of claim 83,
2 wherein the plurality of outer lumens have a plurality of proximal and distal ends
3 coupled with the inner tubular member so as to form a fluted shape multi-lumen
4 balloon between the balloon distal seal end and balloon proximal seal end.

1 85. The multi-lumen balloon radiation centering catheter assembly of claim 83,
2 wherein the inner tubular member extending lengthwise through the central lumen
3 of the multi-lumen balloon is adapted to be attached with a tip rapid exchange
4 guidewire lumen for positioning the catheter within the body vessel.

1 86. The multi-lumen balloon radiation centering catheter assembly of claim 81,
2 further comprising a soft tip coupled to a distal end of the guidewire lumen.

1 87. The multi-lumen balloon radiation centering catheter assembly of claim 85,
2 further comprising a soft tip coupled to a distal end of the tip rapid exchange
3 guidewire lumen.

1 88. The multi-lumen balloon radiation centering catheter assembly of claim 80,
2 further comprising a distal marker and a proximal marker coupled with the radiation

3 source lumen and disposed within the distal seal end and the proximal seal end of
4 the multi-lumen balloon.

1 89. The multi-lumen balloon radiation centering catheter assembly of claim 88,
2 wherein the distal marker is part of a radiation source lumen plug.

1 90. The multi-lumen balloon radiation centering catheter assembly of claim 80,
2 further comprising a radiation source disposed within the radiation source lumen.

1 91. The multi-lumen balloon radiation centering catheter assembly of claim 90,
2 wherein the radiation source comprises a gamma radiation-emitting radiation
3 source.

1 92. The multi-lumen balloon radiation centering catheter assembly of claim 90,
2 wherein the radiation source comprises a beta radiation-emitting radiation source.

1 93. The multi-lumen balloon radiation centering catheter assembly of claim 92,
2 wherein the radiation source comprises phosphorous-32.

1 94. The multi-lumen balloon radiation centering catheter assembly of claim 80,
2 wherein when inflated and engaged with the body vessel, the plurality of outer

3 lumens form straight longitudinal paths that allow for perfusion of blood past the
4 multi-lumen balloon.

1 95. The multi-lumen balloon radiation centering catheter assembly of claim 80,
2 wherein a balloon treatment area is formed between the balloon distal seal end and
3 the balloon proximal seal end.

1 96. The multi-lumen balloon radiation centering catheter assembly of claim 80,
2 wherein the plurality of outer lumens have equal diameters when inflated by the
3 inflation medium.

1 97. The multi-lumen balloon radiation centering catheter assembly of claim 80,
2 wherein the plurality of outer lumens have unequal diameters when inflated by the
3 inflation medium.

1 98. The multi-lumen balloon radiation centering catheter assembly of claim 80,
2 wherein the catheter shaft is a standard rapid exchange type.

1 99. The multi-lumen balloon radiation centering catheter assembly of claim 80,
2 wherein the catheter shaft is a tip rapid exchange type.

1 100. The multi-lumen balloon radiation centering catheter assembly of claim 80,
2 wherein the catheter shaft is an over-the-wire catheter type.

1 101. The multi-lumen balloon radiation centering catheter assembly of claim 95,
2 wherein the balloon treatment area has a longitudinal length in a range of
3 approximately 10-250 mm.

1 102. The multi-lumen balloon radiation centering catheter assembly of claim 95,
2 wherein the balloon treatment area has a longitudinal length in a range of
3 approximately 18-54 mm.

1 103. The multi-lumen balloon radiation centering catheter assembly of claim 95,
2 wherein the balloon treatment area has a combined diameter in a range of
3 approximately 1.5-10 mm when inflated by the inflation medium.

1 104. The multi-lumen balloon radiation centering catheter assembly of claim 95,
2 wherein the balloon treatment area has a combined diameter in a range of
3 approximately 1.5-4 mm when inflated by the inflation medium.

1 105. The multi-lumen balloon radiation centering catheter assembly of claim 95,
2 wherein the multi-lumen balloon is manufactured from a material selected from the
3 group consisting of resin, nylon and pebax.

1 106. A multi-lumen balloon radiation centering catheter assembly, comprising:
2 - a catheter shaft having a distal end and a proximal end, the catheter shaft
3 comprising an inner tubular member extending lengthwise through an outer
4 tubular member, the inner tubular member adapted for receiving a radiation
5 source lumen for centering of the radiation source within a body vessel; and
6 - means for substantially centering the radiation source lumen radially within
7 the body vessel, the centering means disposed at the catheter distal end and
8 comprising a multi-lumen balloon having a plurality of outer lumens disposed
9 around a central lumen, the plurality of outer lumens integrally coupled with the
10 central lumen, the multi-lumen balloon further comprising a plurality of bores
11 communicating between the central lumen and the plurality of outer lumens to
12 allow an inflation medium to enter and inflate the plurality of outer lumens so as
13 to cause the radiation source lumen to be centered within a body vessel.

1 107. A multi-lumen balloon radiation centering catheter assembly, comprising:
2 - a multi-lumen balloon having a plurality of inflatable outer lumens disposed
3 around a central lumen, the plurality of outer lumens integrally coupled with the
4 central lumen so as to form the multi-lumen balloon having a proximal seal end
5 and a distal seal end, the balloon further comprising a plurality of bores
6 communicating between the central lumen and the plurality of outer lumens; and
7 - an over-the-wire catheter shaft having a proximal end and a distal end, the
8 over-the-wire catheter distal end coupled with the balloon proximal seal end, the

9 over-the-wire catheter shaft comprising an inner tubular member which extends
10 coaxially within an outer tubular member, the inner tubular member adapted for
11 receiving a radiation source lumen, the inner tubular member further adapted for
12 receiving at least one inflation lumen that is in fluid communication with the
13 plurality of outer lumens to allow an inflation medium to inflate the plurality of
14 outer lumens so as to cause the radiation source lumen to be centered within a
15 body vessel.

1 108. A multi-lumen balloon radiation centering catheter assembly, comprising:
2 - a multi-lumen balloon having a plurality of inflatable outer lumens disposed
3 around a central lumen, the plurality of outer lumens integrally coupled with the
4 central lumen so as to form the multi-lumen balloon having a proximal seal end
5 and a distal seal end, the balloon further comprising a plurality of bores
6 communicating between the central lumen and the plurality of outer lumens; and
7 - a standard rapid exchange catheter shaft having a proximal end and a distal
8 end, the standard rapid exchange catheter distal end coupled with the balloon
9 proximal seal end, the standard rapid exchange catheter shaft comprising an
10 inner tubular member which extends coaxially within an outer tubular member,
11 the inner tubular member adapted for receiving a radiation source lumen, the
12 inner tubular member further adapted for receiving at least one inflation lumen
13 that is in fluid communication with the plurality of outer lumens to allow an

14 inflation medium to inflate the plurality of outer lumens so as to cause the
15 radiation source lumen to be centered within a body vessel.

1 109. A multi-lumen balloon radiation centering catheter assembly, comprising:

- 2 - a multi-lumen balloon having a plurality of inflatable outer lumens disposed
3 around a central lumen, the plurality of outer lumens integrally coupled with the
4 central lumen so as to form the multi-lumen balloon having a proximal seal end
5 and a distal seal end, the balloon further comprising a plurality of bores
6 communicating between the central lumen and the plurality of outer lumens; and
7 - a tip rapid exchange catheter shaft having a proximal end and a distal end,
8 the tip rapid exchange catheter distal end coupled with the balloon proximal seal
9 end, the tip rapid exchange catheter shaft comprising an inner tubular member
10 which extends coaxially within an outer tubular member, the inner tubular
11 member adapted for receiving a radiation source lumen, the inner tubular
12 member further adapted for receiving at least one inflation lumen that is in fluid
13 communication with the plurality of outer lumens to allow an inflation medium to
14 inflate the plurality of outer lumens so as to cause the radiation source lumen to
15 be centered within a body vessel.

1 110. A multi-lumen balloon radiation centering catheter assembly, comprising:

- 2 - a multi-lumen balloon having a plurality of inflatable outer lumens disposed
3 around a central lumen, the plurality of outer lumens integrally coupled with the

4 central lumen so as to form the multi-lumen balloon having a slideable proximal
5 seal and a slideable distal seal, the balloon further comprising a plurality of
6 bores communicating between the central lumen and the plurality of outer
7 lumens; and

8 - a catheter shaft having a proximal end and a distal end, the catheter distal
9 end coupled with the balloon slideable proximal seal, the catheter shaft
10 comprising an inner tubular member which extends coaxially within an outer
11 tubular member, the inner tubular member adapted for receiving a radiation
12 source lumen, the inner tubular member further adapted for receiving at least
13 one inflation lumen that is in fluid communication with the plurality of outer
14 lumens to allow an inflation medium to inflate the plurality of outer lumens so as
15 to cause the radiation source lumen to be centered within a body vessel.

1

2 111. A multi-lumen balloon radiation centering catheter assembly, comprising:

3 - a multi-lumen balloon having a plurality of inflatable outer lumens disposed
4 around a central lumen, the outer lumens integrally coupled with the central
5 lumen so as to form the multi-lumen balloon;
6 - a catheter shaft disposed proximate to the balloon, the catheter shaft including
7 an inner lumen longitudinally extending through at least a portion of the catheter
8 shaft proximate the balloon, the inner lumen adapted for receiving a radiation
9 source lumen, the inner lumen further adapted to receive a guidewire for

- 10 positioning the multi-lumen balloon radiation centering catheter within a body
11 vessel; and
12 - a slideable distal seal disposed distal to the multi-lumen balloon and a slideable
13 proximal seal disposed proximate to the multi-lumen balloon.

1 112. The multi-lumen balloon radiation centering catheter assembly of claim 111,
2 wherein the inner lumen is further adapted for receiving at least one inflation lumen
3 that is in fluid communication with the outer balloon lumens to allow an inflation
4 medium to enter and inflate the outer lumens so as to cause the radiation source
5 lumen to be centered within a body vessel.

1 113. The multi-lumen balloon radiation centering catheter assembly of claim 111,
2 wherein the guidewire lumen is adapted for receiving a guidewire having a
3 guidewire outer diameter, wherein the guidewire extends lengthwise through one of
4 the plurality of outer lumens of the multi-lumen balloon.

1 114. The multi-lumen balloon radiation centering catheter assembly of claim 113,
2 wherein the slideable proximal and distal seals have an inner diameter formed
3 between the multi-lumen balloon and the catheter shaft.

1 115. The multi-lumen balloon radiation centering catheter assembly of claim 114,
2 wherein the guidewire outer diameter is approximately equal to the inner diameter
3 of the slideable proximal and distal seals.

1 116. The multi-lumen balloon radiation centering catheter assembly of claim 111,
2 wherein the radiation source lumen extends lengthwise through the central lumen of
3 the multi-lumen balloon.

1 117. The multi-lumen balloon radiation centering catheter assembly of claim 113,
2 wherein the guidewire is a standard rapid exchange guidewire.

1 118. The multi-lumen balloon radiation centering catheter assembly of claim 112,
2 wherein the slideable distal and proximal seals are formed such that the guidewire
3 rotates and axially slides relative to the catheter shaft while maintaining the inflation
4 medium within the multi-lumen balloon radiation centering catheter assembly.

1 119 The multi-lumen balloon radiation centering catheter assembly of claim 111,
2 further comprising a distal marker and a proximal marker coupled with the radiation
3 source lumen and disposed within a distal seal end and a proximal seal end of the
4 multi-lumen balloon.

1 120. The multi-lumen balloon radiation centering catheter assembly of claim 119,
2 wherein the distal marker is part of a source lumen plug.

1 121. The multi-lumen balloon radiation centering catheter assembly of claim 111,
2 wherein the radiation source lumen is adapted for receiving a radiation source.

1 122. The multi-lumen balloon radiation centering catheter assembly of claim 121,
2 wherein the radiation source comprises a gamma radiation-emitting radiation
3 source.

1 123. The multi-lumen balloon radiation centering catheter assembly of claim 121,
2 wherein the radiation source comprises a beta radiation-emitting radiation source.

1 124. The multi-lumen balloon radiation centering catheter assembly of claim 123,
2 wherein the radiation source comprises phosphorous-32.

1 125. The multi-lumen balloon radiation centering catheter assembly of claim 111,
2 wherein when inflated and engaged with the body vessel, the plurality of outer
3 lumens form straight longitudinal paths that allow for perfusion of blood past the
4 multi-lumen balloon.

1 126. The multi-lumen balloon radiation centering catheter assembly of claim 119,
2 wherein a balloon treatment area is formed between the balloon distal seal end and
3 the balloon proximal seal end.

1 127. The multi-lumen balloon radiation centering catheter assembly of claim 111,
2 wherein the plurality of outer lumens have equal diameters when inflated by an
3 inflation medium.

1 128. The multi-lumen balloon radiation centering catheter assembly of claim 111,
2 wherein the plurality of outer lumen have unequal diameters when inflated by an
3 inflation medium.

1 129. The multi-lumen balloon radiation centering catheter assembly of claim 126,
2 wherein the balloon treatment area has a longitudinal length in a range of
3 approximately 10-250 mm.

1 130. The multi-lumen balloon radiation centering catheter assembly of claim 126,
2 wherein the balloon treatment area has a longitudinal length in a range of
3 approximately 18-54 mm.

1 131. The multi-lumen balloon radiation centering catheter assembly of claim 126,
2 wherein the balloon treatment area has a combined diameter in a range of
3 approximately 1.5-10 mm when inflated by an inflation medium.

1 132. The multi-lumen balloon radiation centering catheter assembly of claim 126,
2 wherein the balloon treatment area has a combined diameter in a range of
3 approximately 1.5-4 mm when inflated by an inflation medium.

1 133. The multi-lumen balloon radiation centering catheter assembly of claim 113,
2 wherein the slideable distal and proximal seals further include a hydrogel material
3 disposed between the guidewire and the slideable distal and proximal seals.

1 134. The multi-lumen balloon radiation centering catheter assembly of claim 113,
2 wherein the slideable distal and proximal seals further include an O-ring disposed
3 between the guidewire and the slideable distal and proximal seals.

1 135. A multi-lumen balloon radiation centering catheter assembly, comprising:
2 - a multi-lumen balloon having a plurality of inflatable outer lumens disposed
3 around a central lumen, the plurality of outer lumens integrally coupled with the
4 central lumen so as to form the multi-lumen balloon; and
5 - a catheter shaft disposed proximate to the balloon, the catheter shaft having
6 at least two guidewire exit notches, the catheter shaft further including an inner

7 lumen longitudinally extending through at least a portion of the catheter shaft
8 proximate the balloon and connected to the central lumen, the inner lumen
9 adapted for receiving a radiation source lumen, the inner lumen further adapted
10 for receiving a guidewire for positioning the multi-lumen balloon radiation
11 centering catheter within a body vessel, wherein the guidewire extends
12 lengthwise outside the multi-lumen balloon.

1 136. A multi-lumen balloon radiation centering catheter assembly, comprising:
2 - a multi-lumen balloon having a plurality of inflatable outer lumens disposed
3 around a central lumen, the plurality of outer lumens integrally coupled with the
4 central lumen so as to form the multi-lumen balloon;
5 - at least one marker attached to the multi-lumen balloon; and
6 - a catheter shaft disposed proximate to the balloon, the catheter shaft
7 including an inner lumen longitudinally extending through at least a portion of the
8 catheter shaft proximate the balloon and connected to the central lumen, the
9 inner lumen adapted for receiving a radiation source lumen, the inner lumen
10 further adapted for receiving a guidewire lumen for positioning the multi-lumen
11 balloon radiation centering catheter within a body vessel.

137. A multi-lumen balloon radiation centering catheter assembly, comprising:

- a multi-lumen balloon having a plurality of inflatable outer lumens disposed around a central lumen, the plurality of outer lumens integrally coupled with the central lumen so as to form the multi-lumen balloon;
- at least one marker attached to the multi-lumen balloon using a vapor deposition process; and
- a catheter shaft disposed proximate to the balloon, the catheter shaft including an inner lumen longitudinally extending through at least a portion of the catheter shaft proximate the balloon and connected to the central lumen, the inner lumen adapted for receiving a radiation source lumen, the inner lumen further adapted for receiving a guidewire lumen for positioning the multi-lumen balloon radiation centering catheter within a body vessel.

ABSTRACT OF THE INVENTION

A multi-lumen balloon for use in a fluted balloon centering catheter and method for providing the same. The multi-lumen balloon maintains a radiation source at the center of a cardiovascular artery, has improved blood perfusion capability, and has improved balloon refolding characteristics. The method of fabricating a multi-lumen balloon designed for a radiation centering catheter uses an improved extrusion process that allows the manufacture of the multi-lumen balloon sub-assembly to be done separately from the catheter shaft assembly.

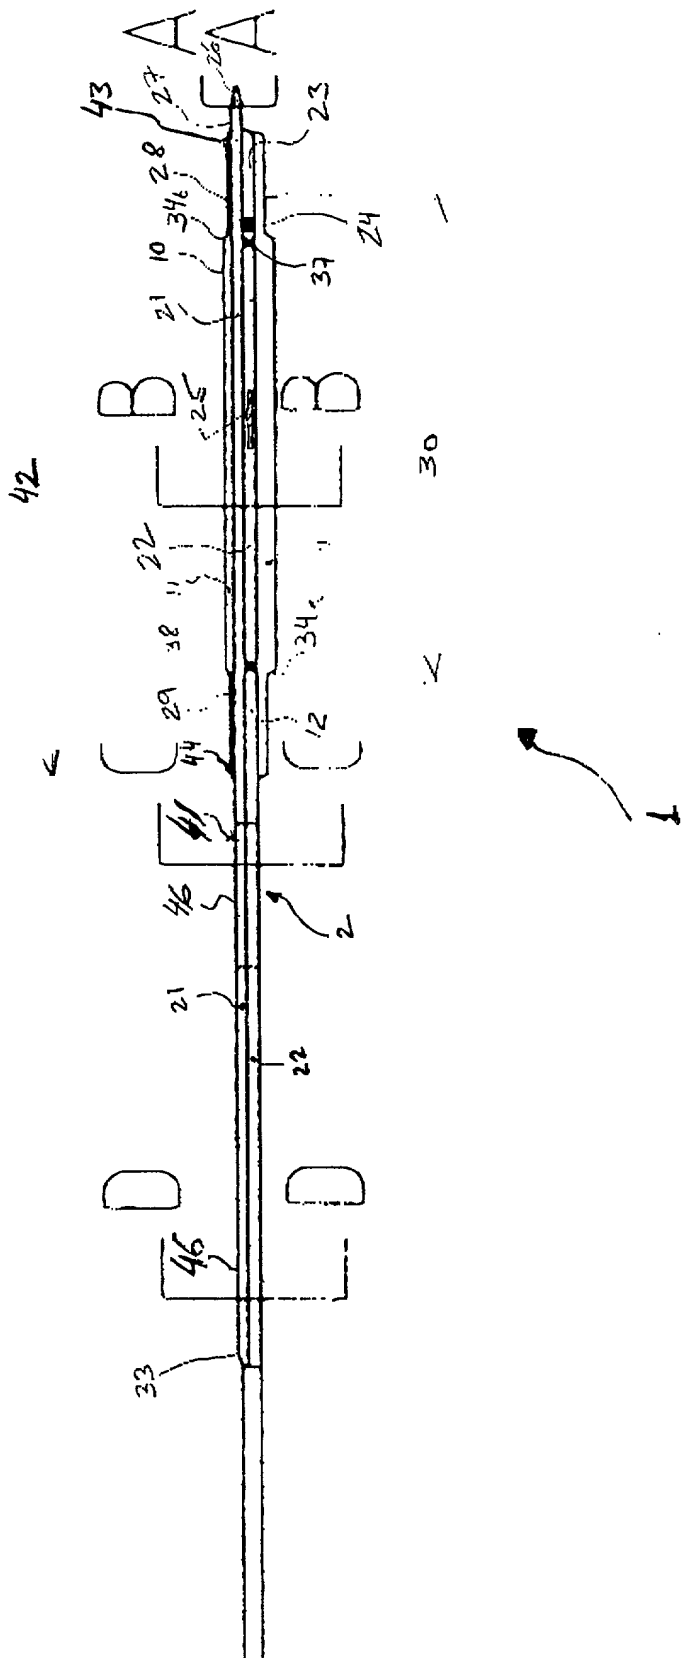


Fig. 1




FIG. 2

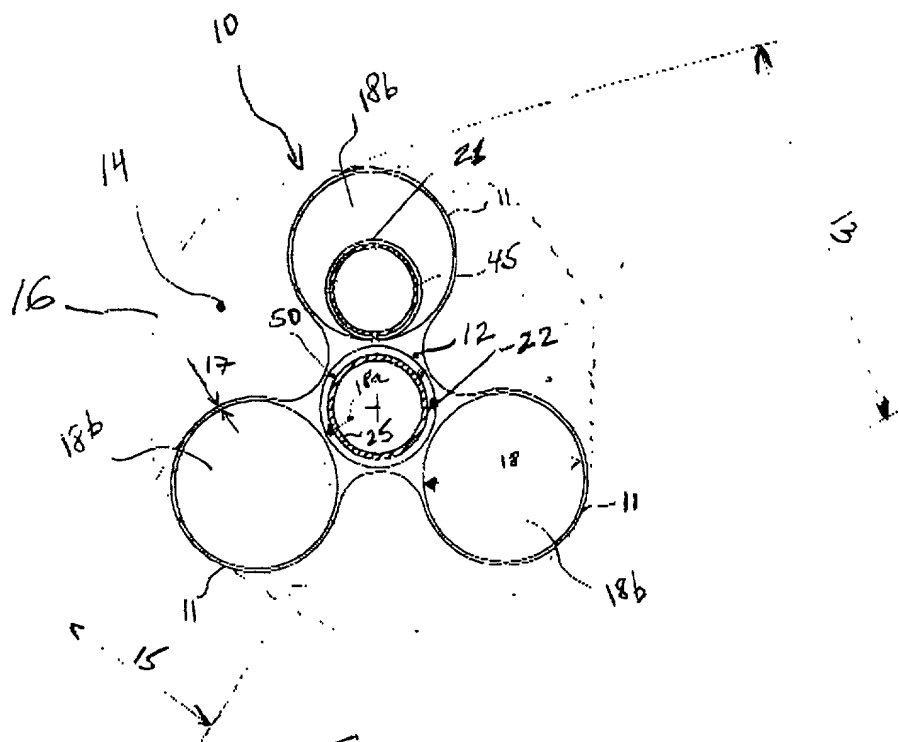


FIG. 3

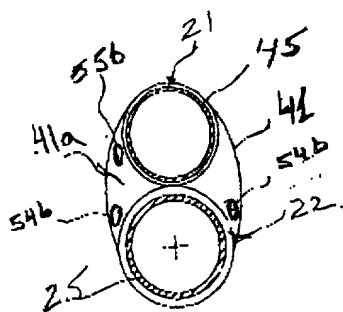


FIG. 4

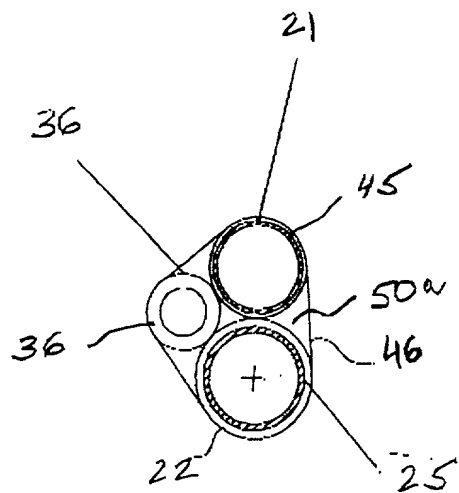


FIG. 5

FIG. 6

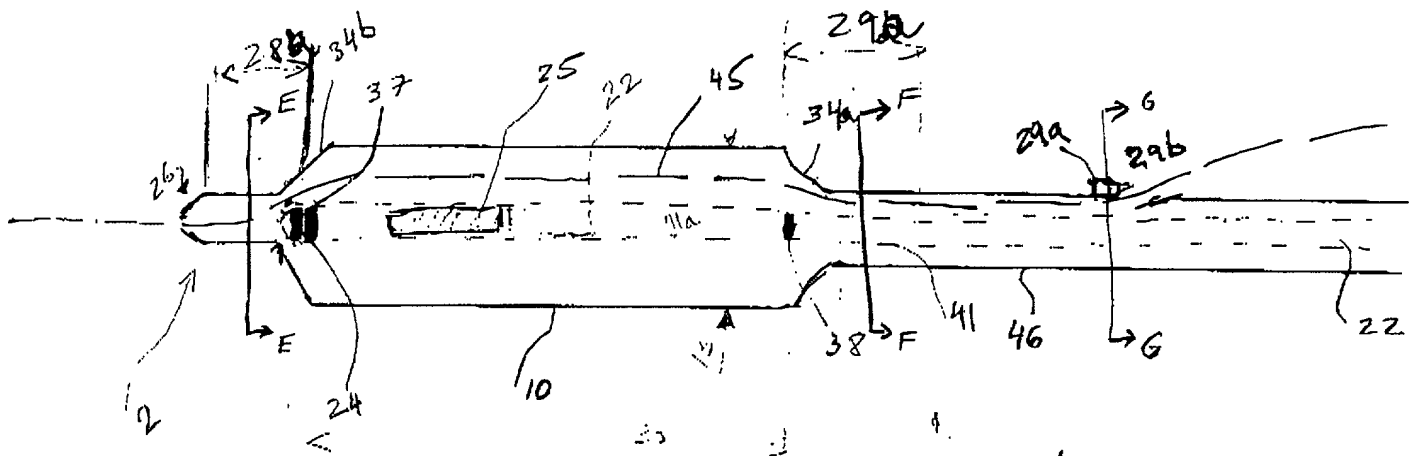


FIG. 7

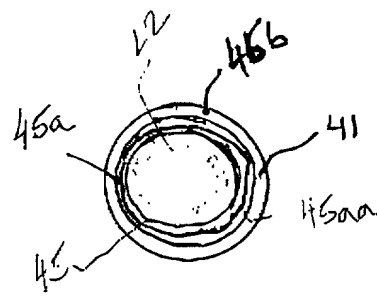


FIG. 8

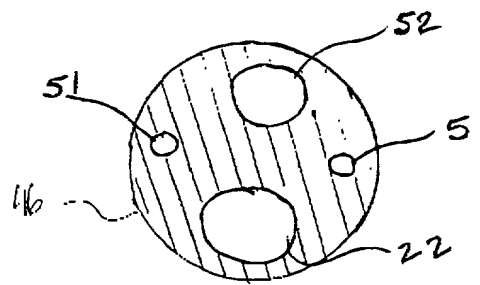
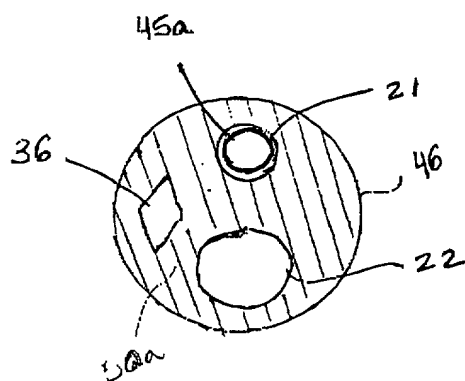


FIG. 9



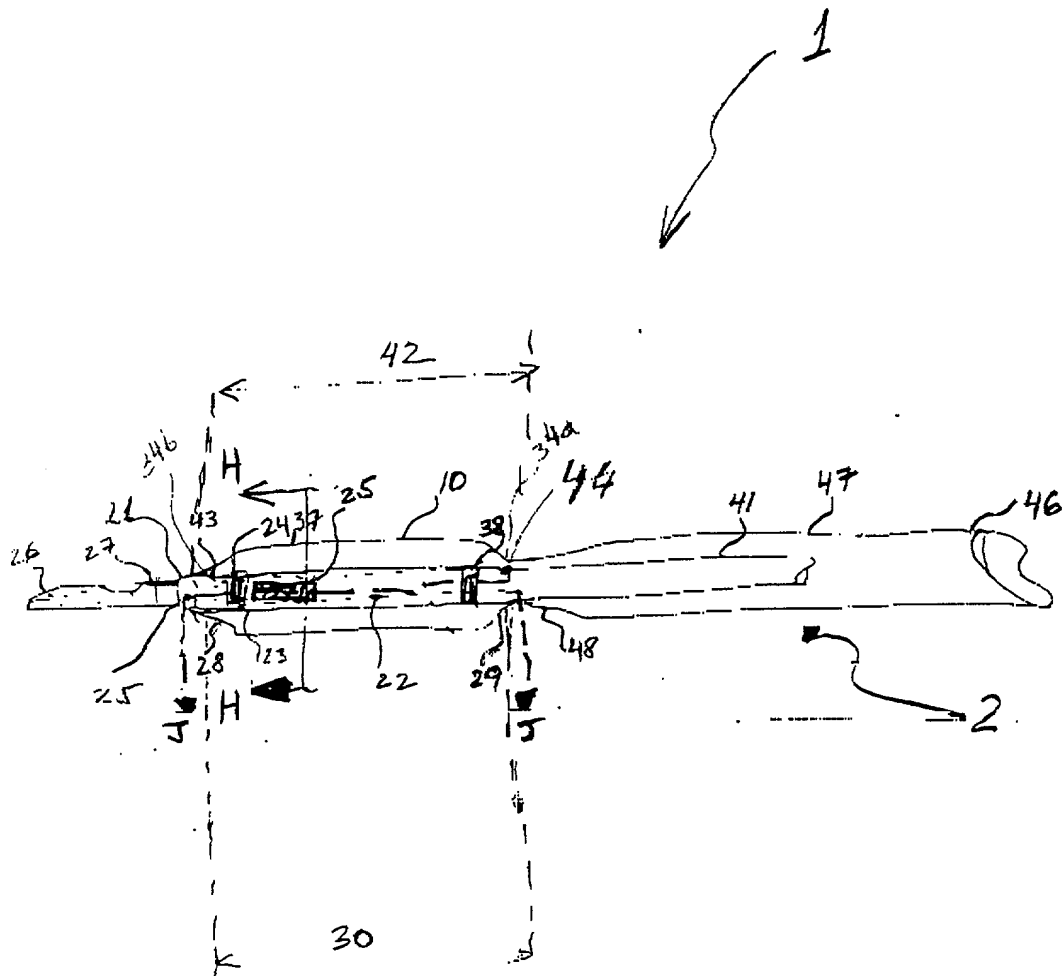


FIG. 10

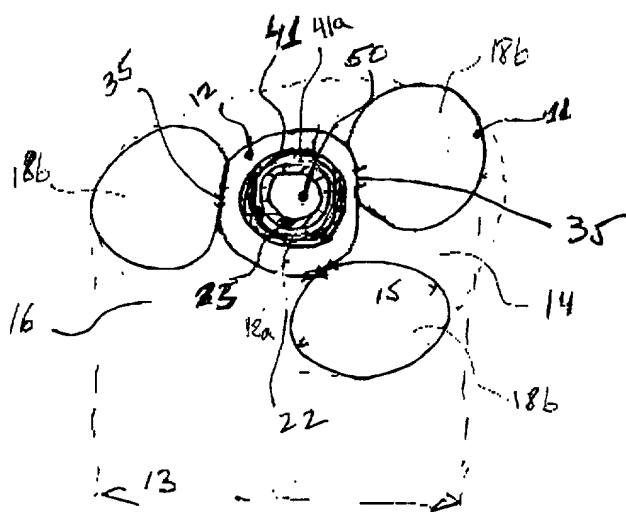


FIG. 11

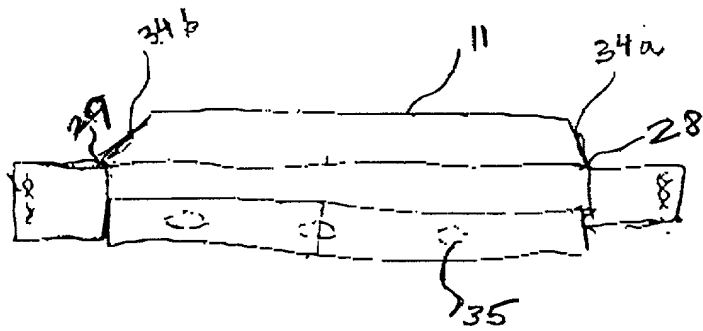


FIG. 12

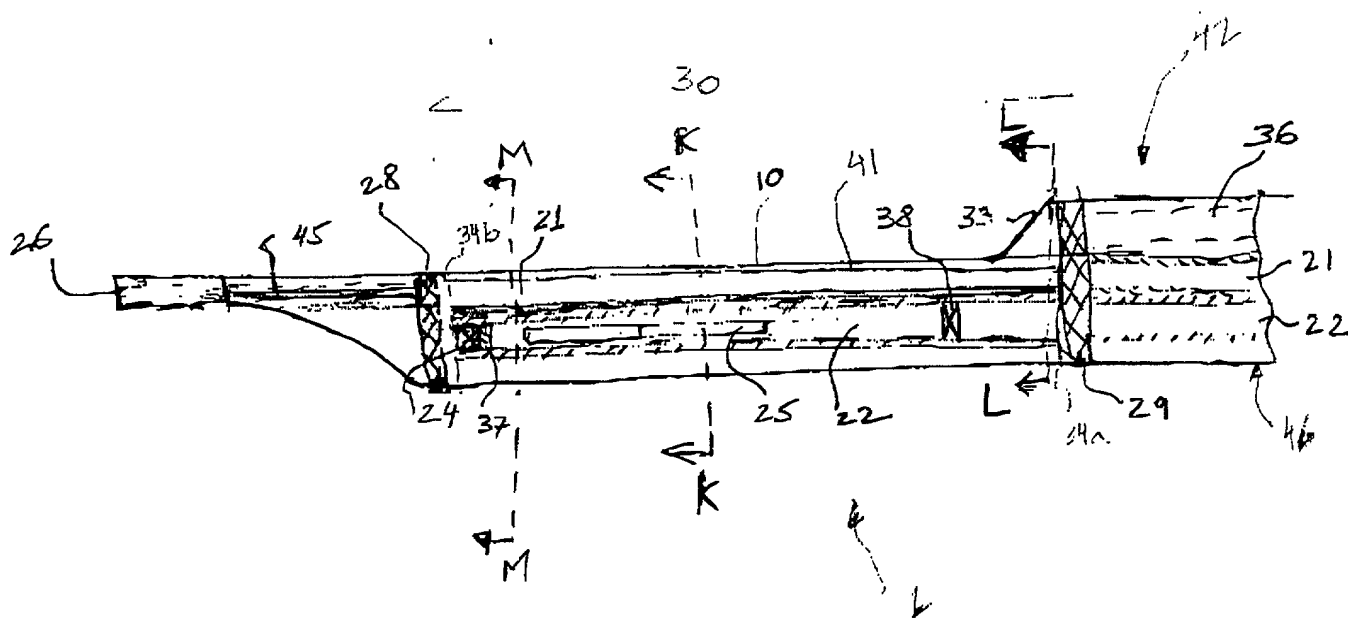


FIG. 13

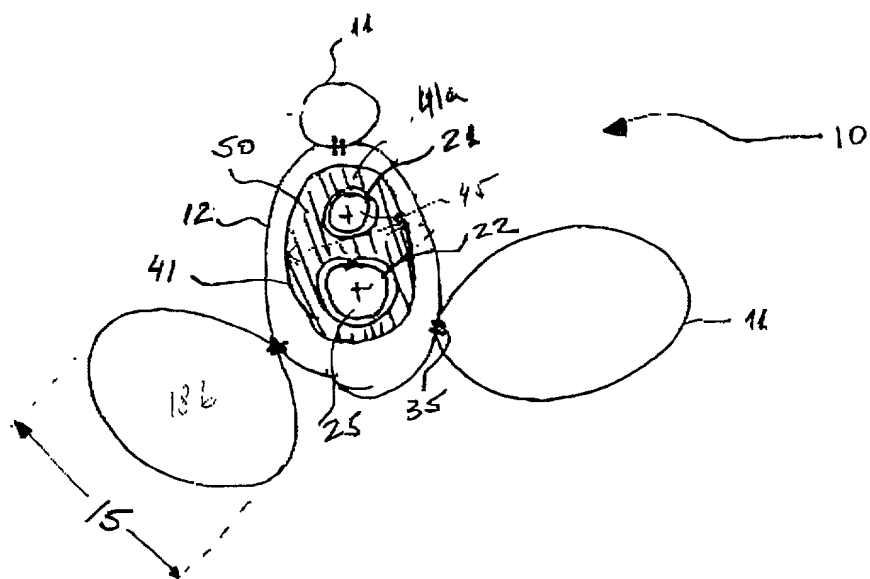


FIG. 14

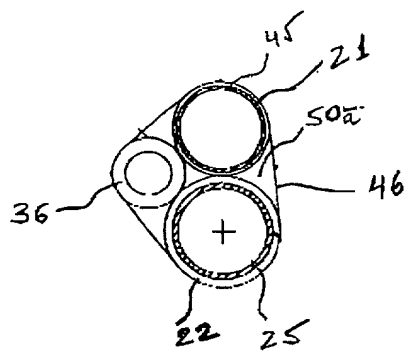
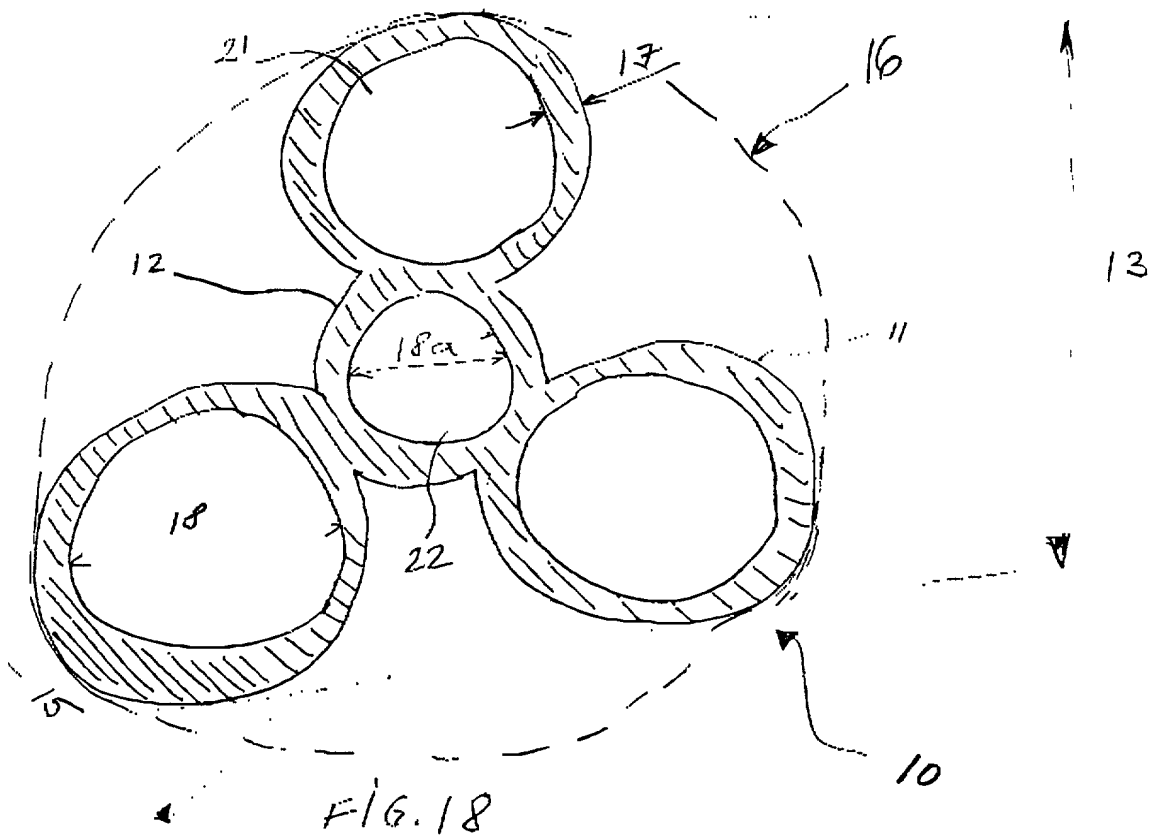
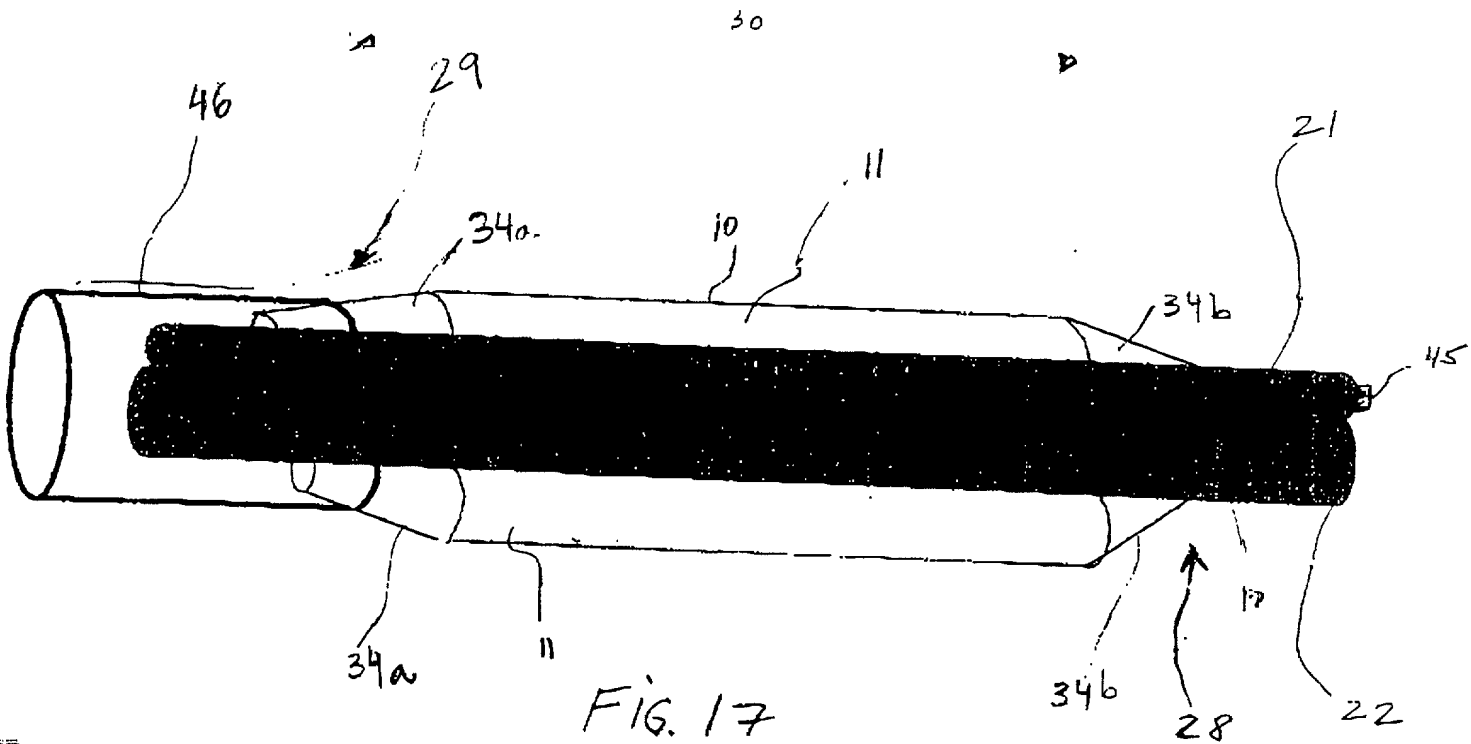


FIG. 15

Fig. 16

009720-18090560



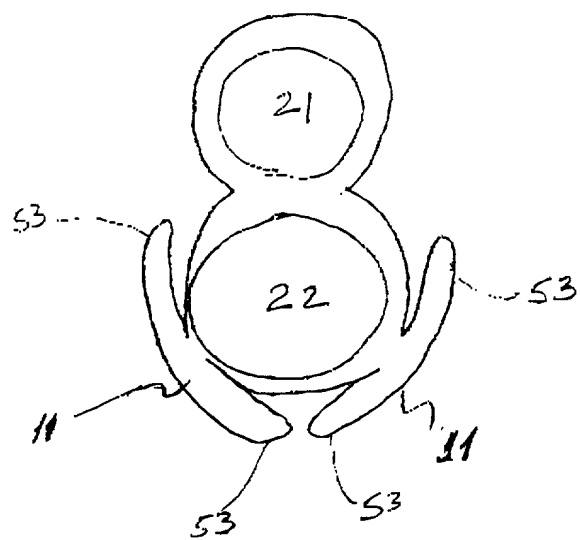


FIG. 19a

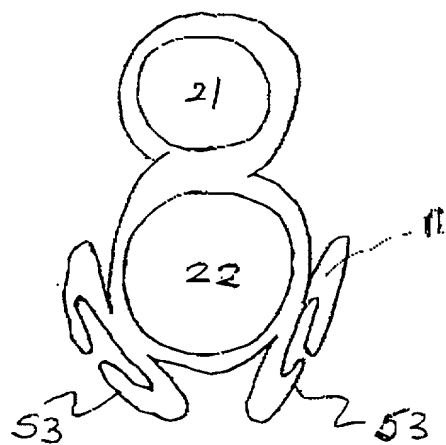


FIG. 19c





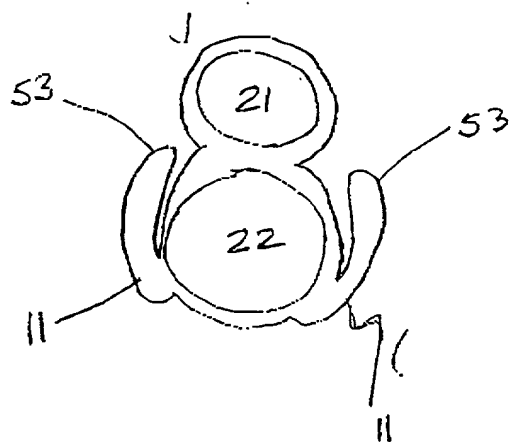


FIG. 19b

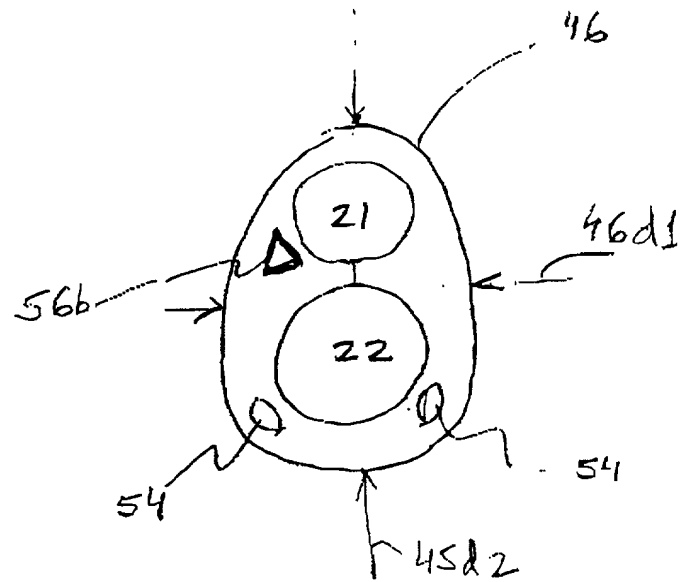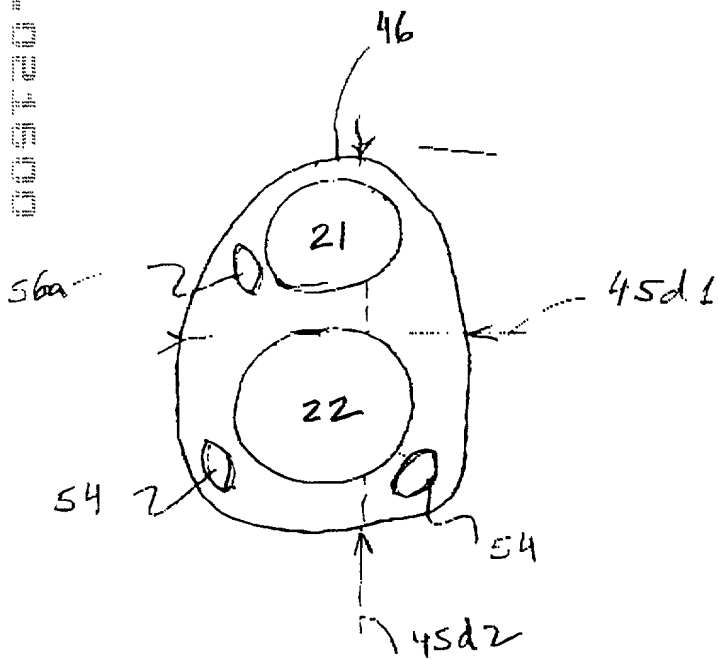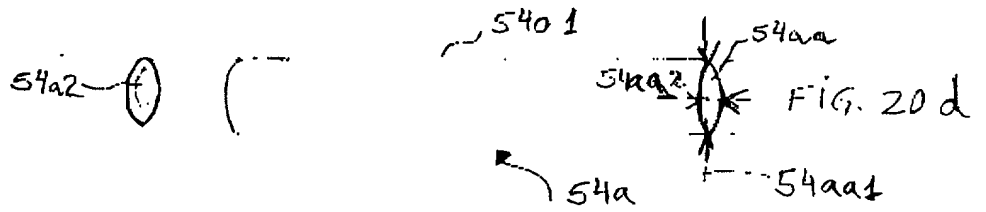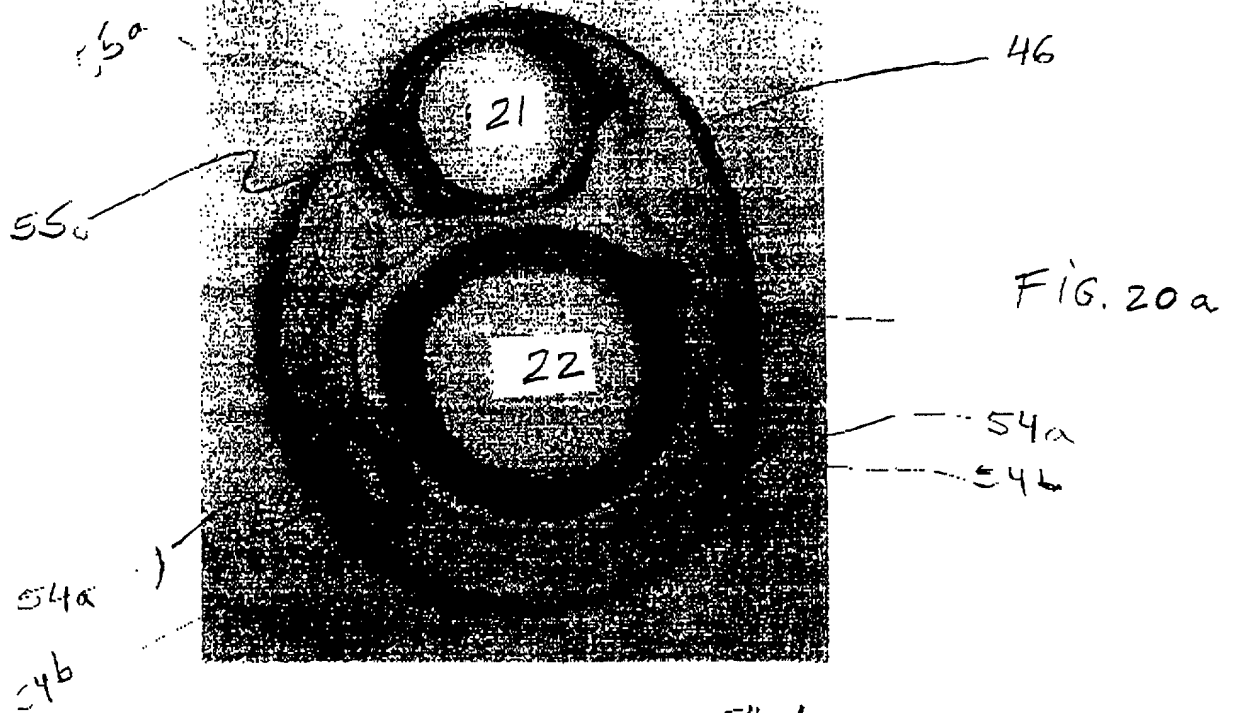

009120-18090560

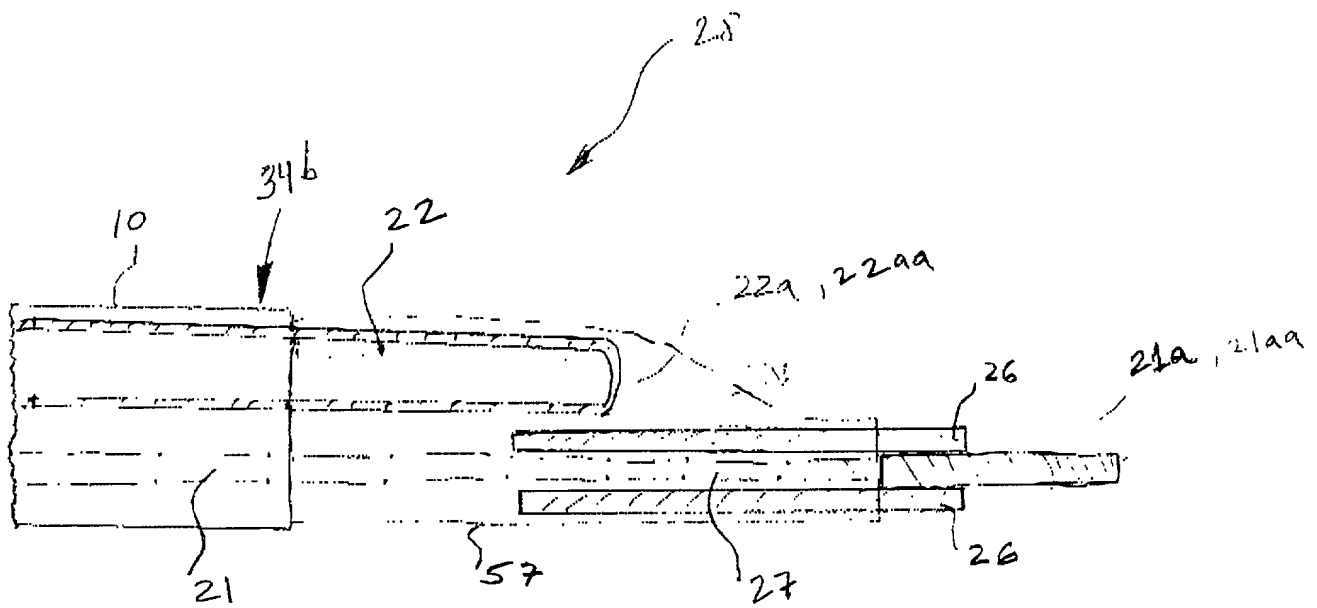




FIG. 21a



FIG. 21b.



FIG. 21c

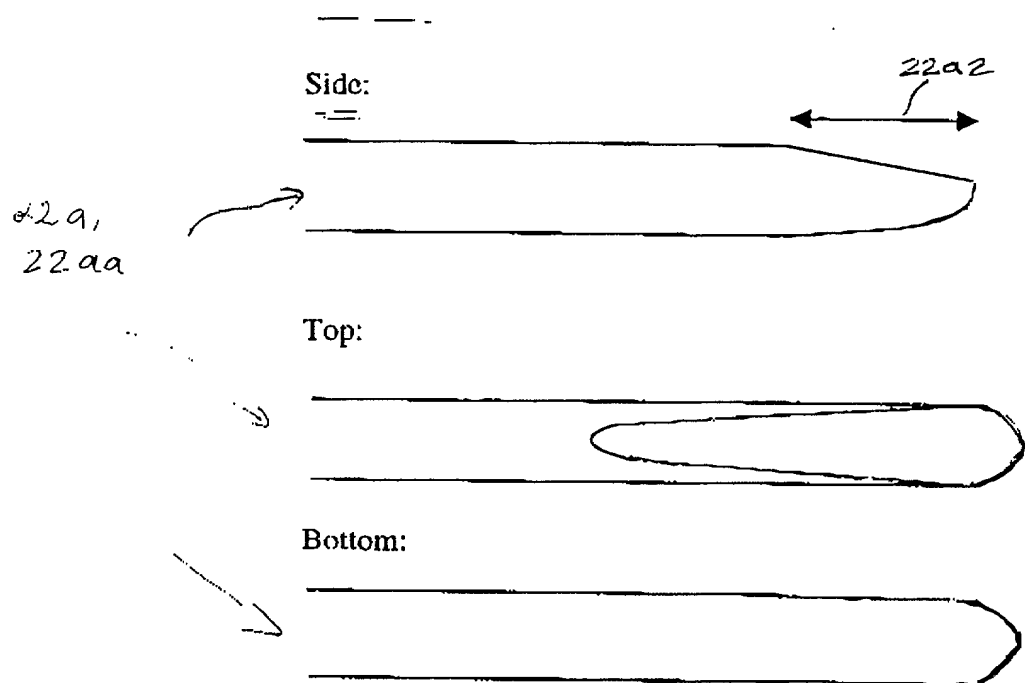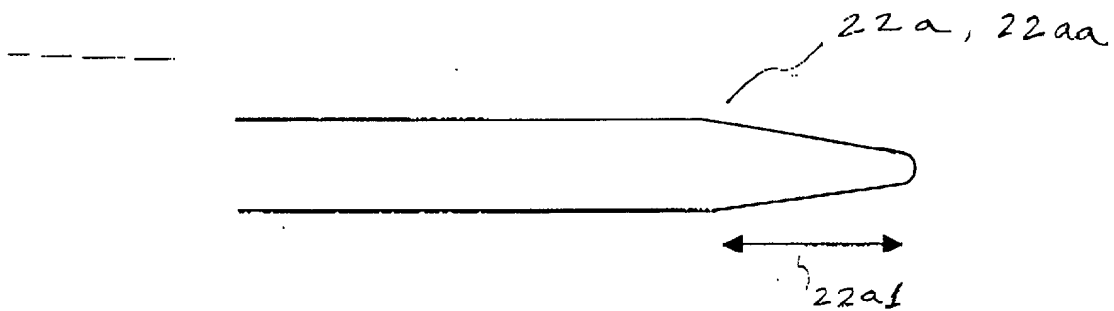

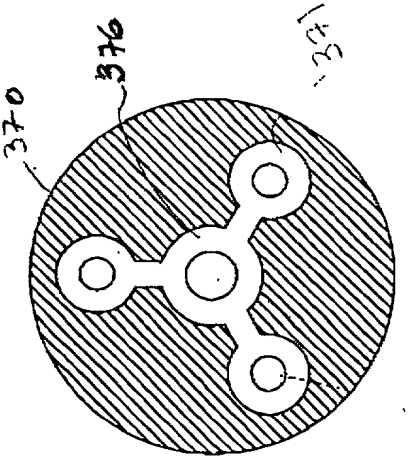
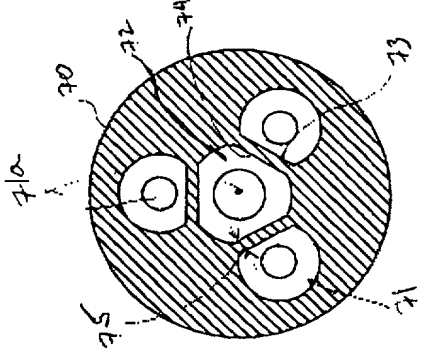
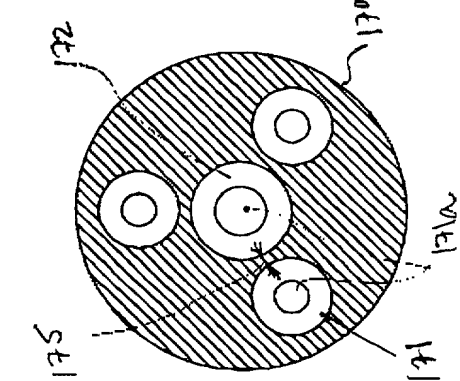
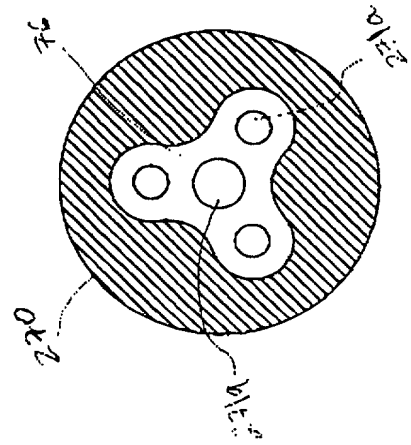
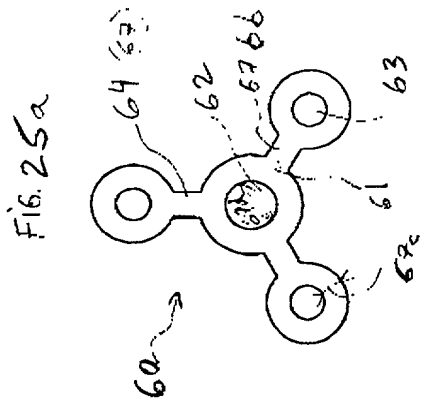
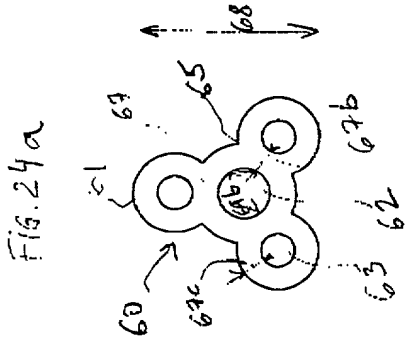
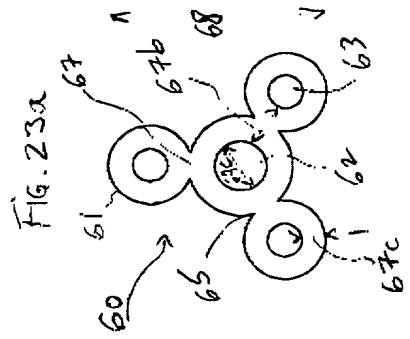
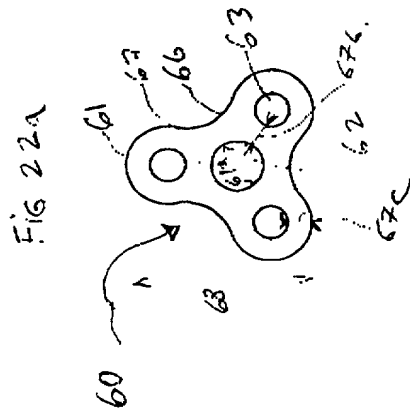


FIG. 22b

FIG. 23b

FIG. 24b

FIG. 25b

FIG. 26

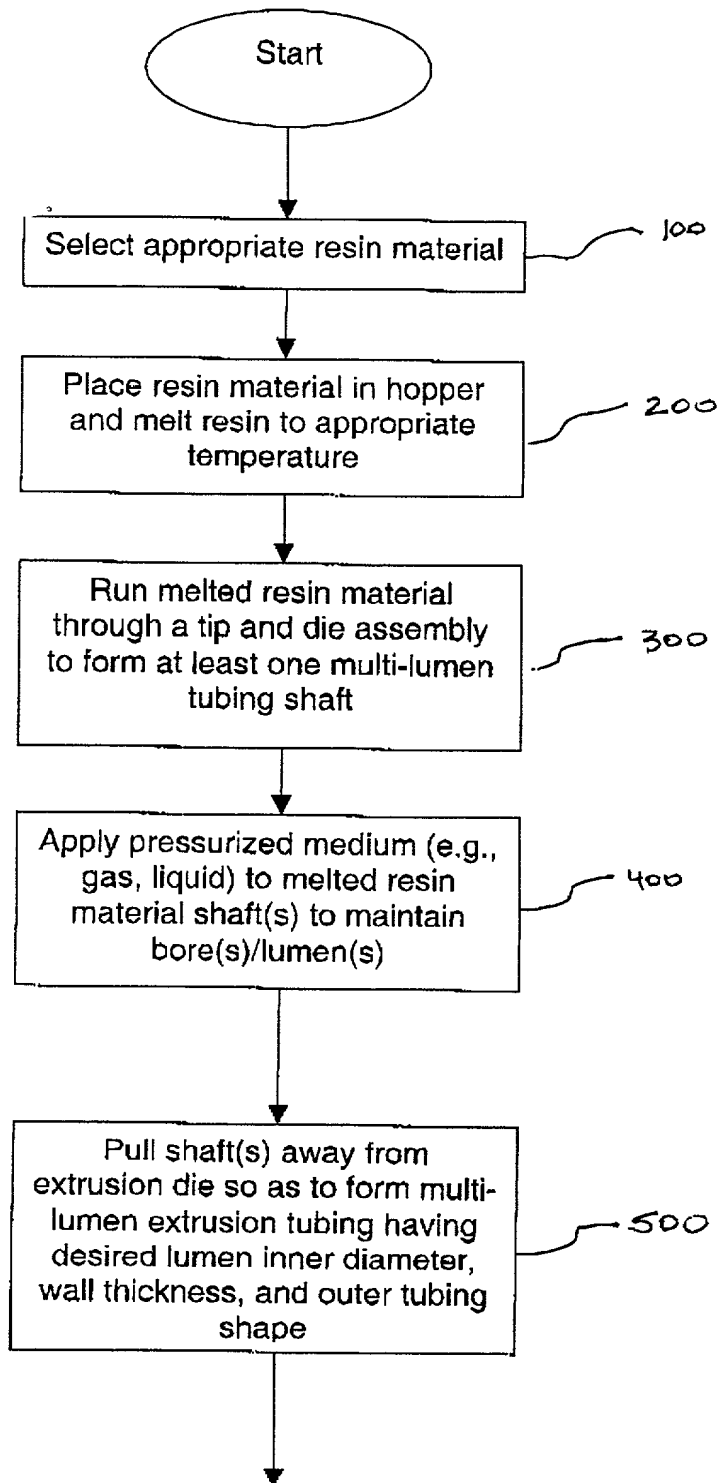
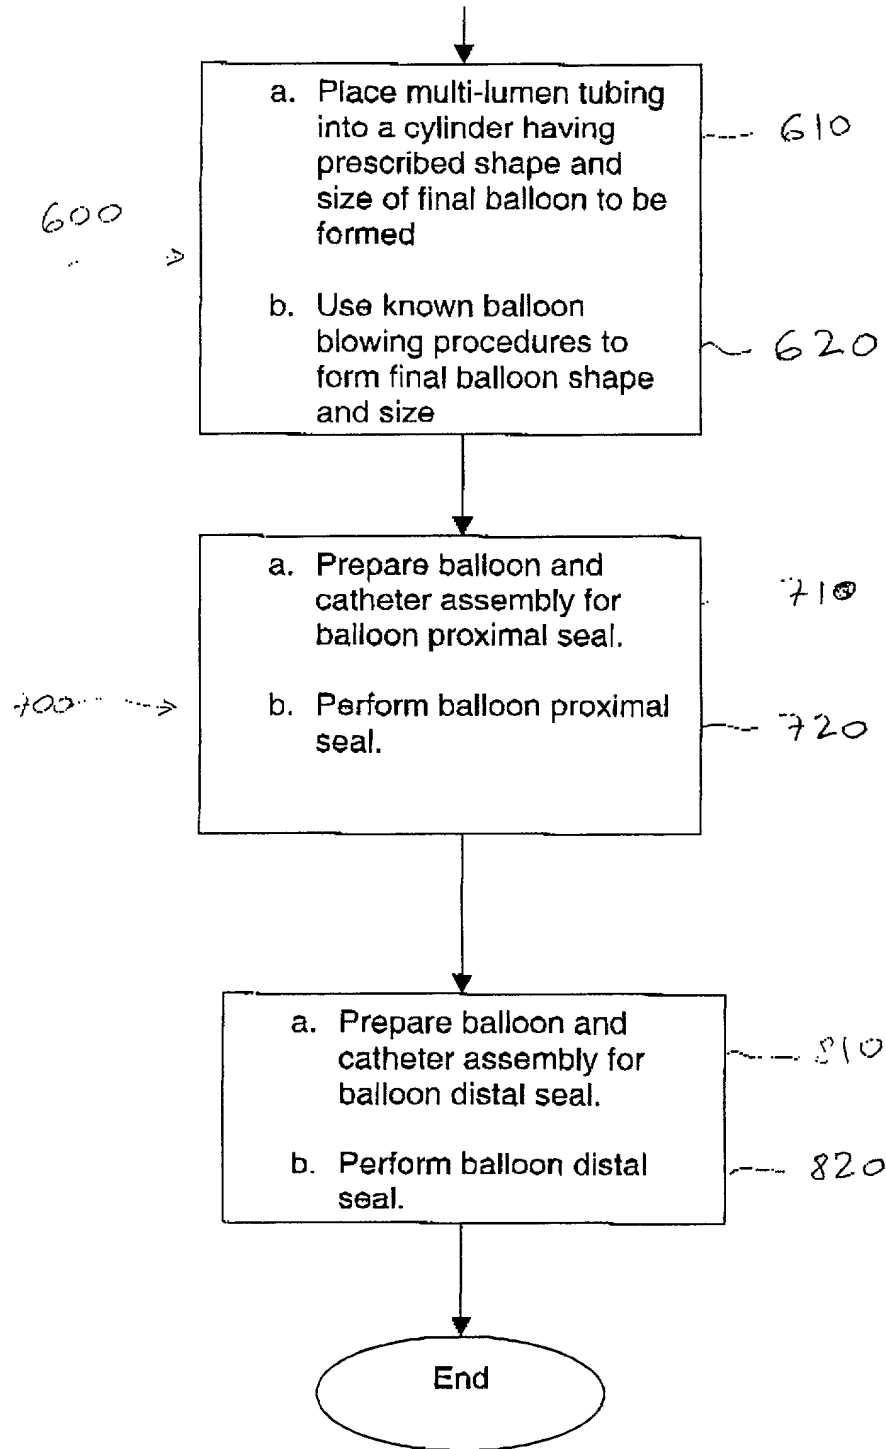


FIG. 26 (cont.)



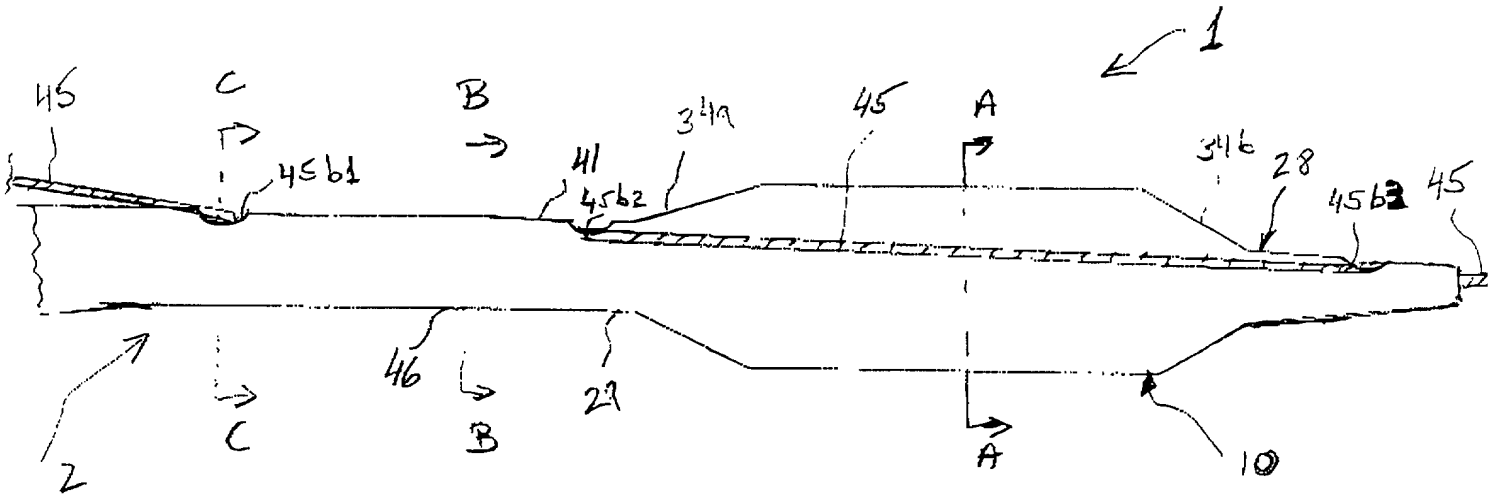


Fig. 27a

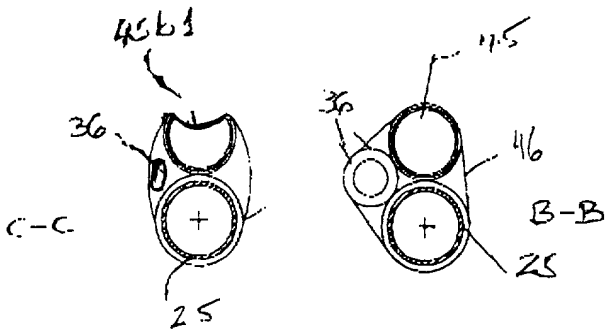


Fig. 27d




Fig. 27c

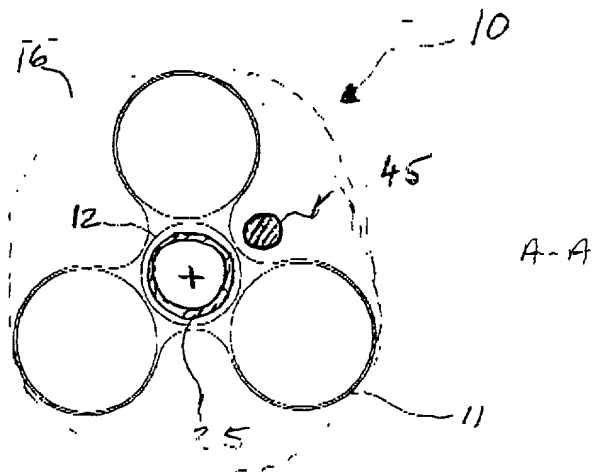


Fig. 27b

009594-02500

DECLARATION AND POWER OF ATTORNEY FOR PATENT APPLICATION
(FOR GUIDANT CORPORATION PATENT APPLICATIONS)

As a below named inventor, I hereby declare that:

My residence, post office address and citizenship are as stated below, next to my name.

I believe I am the original, first, and sole inventor (if only one name is listed below) or an original, first, and joint inventor (if plural names are listed below) of the subject matter which is claimed and for which a patent is sought on the invention entitled

MULTI-LUMEN FLUTED BALLOON RADIATION CENTERING CATHETER

the specification of which

X is attached hereto.
_____ was filed on _____ as
United States Application Number _____
or PCT International Application Number _____
and was amended on _____
(if applicable)

I hereby state that I have reviewed and understand the contents of the above-identified specification, including the claim(s), as amended by any amendment referred to above.

I do not know and do not believe that the claimed invention was ever known or used in the United States of America before my invention thereof, or patented or described in any printed publication in any country before my invention thereof or more than one year prior to this application, that the same was not in public use or on sale in the United States of America more than one year prior to this application, and that the invention has not been patented or made the subject of an inventor's certificate issued before the date of this application in any country foreign to the United States of America on an application filed by me or my legal representatives or assigns more than twelve months (for a utility patent application) or six months (for a design patent application) prior to this application.

I acknowledge the duty to disclose all information known to me to be material to patentability as defined in Title 37, Code of Federal Regulations, Section 1.56.

I hereby claim foreign priority benefits under Title 35, United States Code, Section 119(a)-(d) or 365(b) of any foreign application(s) for patent or inventor's certificate, or 365(a) of any PCT international application which designated at least one country other than the United States of America, listed below and have also identified below any foreign application for patent or inventor's certificate, or of any PCT international application having a filing date before that of the application on which priority is claimed:

<u>Prior Foreign Application(s)</u>			<u>Priority Claimed</u>	
<u>(Number)</u>	<u>(Country)</u>	<u>(Day/Month/Year Filed)</u>	<u>Yes</u>	<u>No</u>
<u>(Number)</u>	<u>(Country)</u>	<u>(Day/Month/Year Filed)</u>	<u>Yes</u>	<u>No</u>
<u>(Number)</u>	<u>(Country)</u>	<u>(Day/Month/Year Filed)</u>	<u>Yes</u>	<u>No</u>
<u>(Number)</u>	<u>(Country)</u>	<u>(Day/Month/Year Filed)</u>	<u>Yes</u>	<u>No</u>

I hereby claim the benefit under title 35, United States Code, Section 119(e) of any United States provisional application(s) listed below

(Application Number)

Filing Date

(Application Number)

Filing Date

I hereby claim the benefit under Title 35, United States Code, Section 120 of any United States application(s), or 365(c) of any PCT International application designating the United states of America, listed below and, insofar as the subject matter of each of the claims of this application is not disclosed in the prior United States or PCT International application in the manner provided by the first paragraph of Title 35, United States Code, Section 112, I acknowledge the duty to disclose all information known to me to be material to patentability as defined in Title 37, Code of Federal Regulations, Section 1.56 which became available between the filing date of the prior application and the national or PCT international filing date of this application:

(U.S. Parent Application or
PCT Parent No.)

Parent Filing Date

(Status -- patented,
pending, abandoned)

Parent Patent No.
(if applicable)

(U.S. Parent Application or
PCT Parent No.)

Parent Filing Date

(Status -- patented,
pending, abandoned)

Parent Patent No.
(if applicable)

I hereby appoint the persons listed on Appendix A hereto (which is incorporated by reference and a part of this document) as my respective patent attorneys and patent agents, with full power of substitution and revocation, to prosecute this application and to transact all business in the Patent and Trademark Office connected herewith.

Send correspondence to Darren J. Milliken , BLAKELY, SOKOLOFF, TAYLOR &
(Name of Attorney or Agent)

ZAFMAN LLP, 12400 Wilshire Boulevard, 7th Floor, Los Angeles, California 90025 and
direct telephone calls to Darren J. Milliken , (408) 720-8300.
(Name of Attorney or Agent)

I hereby declare that all statements made herein of my own knowledge are true and that all statements made on information and belief are believed to be true; and further that these statements were made with the knowledge that willful false statements and the like so made are punishable by fine or imprisonment, or both, under Section 1001 of Title 18 of the United States Code and that such willful false statements may jeopardize the validity of the application or any patent issued thereon.

Full Name of Sole/First Inventor Jessica Chiu

Inventor's Signature _____ Date _____

Residence Palo Alto, California Citizenship USA
(City, State) (Country)

Post Office Address 3790 El Camino Real, #221
Palo Alto, California 94306

Full Name of Second/Joint Inventor Manolo F. Lumaig

Inventor's Signature _____ Date _____

Residence San Jose, California Citizenship USA
(City, State) (Country)

Post Office Address 1259 Lodestone Drive
San Jose, California 95132

Full Name of Third/Joint Inventor Eric D. Peterson

Inventor's Signature _____ Date _____

Residence Fremont, California Citizenship USA
(City, State) (Country)

Post Office Address 46820 Cloverleaf Court
Fremont, California 94539

APPENDIX A

William E. Alford, Reg. No. 37,764; Farzad E. Amini, Reg. No. P42,261; Aloysius T. C. AuYeung, Reg. No. 35,432; William Thomas Babbitt, Reg. No. 39,591; Carol F. Barry, Reg. No. 41,600; Jordan Michael Becker, Reg. No. 39,602; Bradley J. Bereznak, Reg. No. 33,474; Michael A. Bernadicou, Reg. No. 35,934; Roger W. Blakely, Jr., Reg. No. 25,831; Gregory D. Caldwell, Reg. No. 39,926; Ronald C. Card, Reg. No. P44,587; Thomas M. Coester, Reg. No. 39,637; Stephen M. De Klerk, under 37 C.F.R. § 10.9(b); Michael Anthony DeSanctis, Reg. No. 39,957; Daniel M. De Vos, Reg. No. 37,813; Robert Andrew Diehl, Reg. No. 40,992; Matthew C. Fagan, Reg. No. 37,542; Tarek N. Fahmi, Reg. No. 41,402; James Y. Go, Reg. No. 40,621; James A. Henry, Reg. No. 41,064; Willmore F. Holbrow III, Reg. No. P41,845; Sheryl Sue Holloway, Reg. No. 37,850; George W. Hoover II, Reg. No. 32,992; Eric S. Hyman, Reg. No. 30,139; William W. Kidd, Reg. No. 31,772; Erica W. Kuo, Reg. No. 42,775; Michael J. Mallie, Reg. No. 36,591; Andre L. Marais, under 37 C.F.R. § 10.9(b); Paul A. Mendonsa, Reg. No. 42,879; Darren J. Milliken, Reg. No. 42,004; Lisa A. Norris, Reg. No. P44,976; Chun M. Ng, Reg. No. 36,878; Thien T. Nguyen, Reg. No. 43,835; Thinh V. Nguyen, Reg. No. 42,034; Dennis A. Nicholls, Reg. No. 42,036; Daniel E. Ovanezian, Reg. No. 41,236; William F. Ryann, Reg. No. 44,313; James H. Salter, Reg. No. 35,668; William W. Schaal, Reg. No. 39,018; James C. Scheller, Reg. No. 31,195; Jeffrey Sam Smith, Reg. No. 39,377; Maria McCormack Sobrino, Reg. No. 31,639; Stanley W. Sokoloff, Reg. No. 25,128; Judith A. Szepesi, Reg. No. 39,393; Vincent P. Tassinari, Reg. No. 42,179; Edwin H. Taylor, Reg. No. 25,129; John F. Travis, Reg. No. 43,203; George G. C. Tseng, Reg. No. 41,355; Joseph A. Twarowski, Reg. No. 42,191; Lester J. Vincent, Reg. No. 31,460; Glenn E. Von Tersch, Reg. No. 41,364; John Patrick Ward, Reg. No. 40,216; Charles T. J. Weigell, Reg. No. 43,398; Kirk D. Williams, Reg. No. 42,229; James M. Wu, Reg. No. P45,241; Steven D. Yates, Reg. No. 42,242; Ben J. Yorks, Reg. No. 33,609; and Norman Zafman, Reg. No. 26,250; my patent attorneys, and Andrew C. Chen, Reg. No. 43,544; Justin M. Dillon, Reg. No. 42,486; Paramita Ghosh, Reg. No. 42,806; and Sang Hui Kim, Reg. No. 40,450; my patent agents, of BLAKELY, SOKOLOFF, TAYLOR & ZAFMAN LLP, with offices located at 12400 Wilshire Boulevard, 7th Floor, Los Angeles, California 90025, telephone (310) 207-3800, and James R. Thein, Reg. No. 31,710, my patent attorney; with full power of substitution and revocation, to prosecute this application and to transact all business in the Patent and Trademark Office connected herewith.

I also hereby appoint Earl A. Bright II, Reg. No. 37,045; Ronald D. Devore, Reg. No. 39,958; Thomas A. Hassing, Reg. No. 36,159; Tim L. Kitchen, Reg. No. 41,900; Philip S. Yip, Reg. No. 37,265; my attorneys of Guidant Corporation located at 3200 Lakeside Drive, Santa Clara, CA 95054, telephone (408) 845-3000; and Guidant Corporation located at 1525 O'Brien Drive, Menlo Park, CA 94025, telephone (650) 470-6200; with full power of substitution and revocation, to prosecute this application and to transact all business in the Patent and Trademark Office connected herewith.

APPENDIX B

Title 37, Code of Federal Regulations, Section 1.56 Duty to Disclose Information Material to Patentability

(a) A patent by its very nature is affected with a public interest. The public interest is best served, and the most effective patent examination occurs when, at the time an application is being examined, the Office is aware of and evaluates the teachings of all information material to patentability. Each individual associated with the filing and prosecution of a patent application has a duty of candor and good faith in dealing with the Office, which includes a duty to disclose to the Office all information known to that individual to be material to patentability as defined in this section. The duty to disclosure information exists with respect to each pending claim until the claim is cancelled or withdrawn from consideration, or the application becomes abandoned. Information material to the patentability of a claim that is cancelled or withdrawn from consideration need not be submitted if the information is not material to the patentability of any claim remaining under consideration in the application. There is no duty to submit information which is not material to the patentability of any existing claim. The duty to disclose all information known to be material to patentability is deemed to be satisfied if all information known to be material to patentability of any claim issued in a patent was cited by the Office or submitted to the Office in the manner prescribed by §§1.97(b)-(d) and 1.98. However, no patent will be granted on an application in connection with which fraud on the Office was practiced or attempted or the duty of disclosure was violated through bad faith or intentional misconduct. The Office encourages applicants to carefully examine:

- (1) Prior art cited in search reports of a foreign patent office in a counterpart application, and
 - (2) The closest information over which individuals associated with the filing or prosecution of a patent application believe any pending claim patentably defines, to make sure that any material information contained therein is disclosed to the Office.
- (b) Under this section, information is material to patentability when it is not cumulative to information already of record or being made of record in the application, and
- (1) It establishes, by itself or in combination with other information, a prima facie case of unpatentability of a claim; or
 - (2) It refutes, or is inconsistent with, a position the applicant takes in:
 - (i) Opposing an argument of unpatentability relied on by the Office, or
 - (ii) Asserting an argument of patentability.

A prima facie case of unpatentability is established when the information compels a conclusion that a claim is unpatentable under the preponderance of evidence, burden-of-proof standard, giving each term in the claim its broadest reasonable construction consistent with the specification, and before any consideration is given to evidence which may be submitted in an attempt to establish a contrary conclusion of patentability.

(c) Individuals associated with the filing or prosecution of a patent application within the meaning of this section are:

- (1) Each inventor named in the application;
 - (2) Each attorney or agent who prepares or prosecutes the application; and
 - (3) Every other person who is substantively involved in the preparation or prosecution of the application and who is associated with the inventor, with the assignee or with anyone to whom there is an obligation to assign the application.
- (d) Individuals other than the attorney, agent or inventor may comply with this section by disclosing information to the attorney, agent, or inventor.